




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 7 : A61B 17/34, A61M 29/00		A1	(11) International Publication Number: WO 00/18306
			(43) International Publication Date: 6 April 2000 (06.04.00)
<p>(21) International Application Number: PCT/US99/21866</p> <p>(22) International Filing Date: 21 September 1999 (21.09.99)</p> <p>(30) Priority Data: 09/160,882 25 September 1998 (25.09.98) US</p> <p>(71) Applicant (for all designated States except US): SDGI HOLDINGS, INC. [US/US]; Suite 508, 300 Delaware Avenue, Wilmington, DE 19801 (US).</p> <p>(72) Inventors; and</p> <p>(75) Inventors/Applicants (for US only): FOLEY, Kevin, T. [US/US]; 2877 Keasler Circle West, Germantown, TN 38139 (US). SMITH, Maurice, M. [US/US]; 9285 Oak Knoll Cove, Cordova, TN 38018 (US). CLAYTON, John, B. [US/US]; 1405 Stoneham, Superior, CO 80027 (US). MOCTEZUMA, Joseph [US/US]; 3791 St. Philip, Memphis, TN 38133 (US). ROEHM, Thomas, E., III [US/US]; P.O. Box 1372, 410 Highway 59, Braden, TN 38010 (US).</p> <p>(74) Agents: COLLIER, Douglas, A. et al.; Woodard, Emhardt, Naughton, Moriarty & Mcnett, Suite 3700, Bank One Center/Tower, 111 Monument Circle, Indianapolis, IN 46204 (US).</p>		<p>(81) Designated States: AE, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CR, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published With international search report.</p>	

(54) Title: DEVICES AND METHODS FOR PERCUTANEOUS SURGERY

(57) Abstract

Devices and methods for performing percutaneous surgery under direct visualization through a single cannula are shown. A device includes an elongated cannula (20) sized for percutaneous introduction that defines a working channel (21) between its ends. The working channel (21) is sized to receive one or more surgical tools therethrough. A clamp assembly (350, 400) is engaged to the outer surface of the cannula (20). The clamp assembly (350, 400) includes a viewing element receiving portion (390) and a viewing element (310) includes a clamp assembly engaging portion for removably engaging the viewing element (310) to the clamp assembly (350, 400). In one embodiment, the receiving portion (390) defines a receptacle for receiving a dovetail (330) included on the engaging portion of the viewing element (310). The receiving portion (390) may also include a pivotable clip (340) for removably engaging a protuberance (335) of the engaging portion. The clamp (350, 400) includes a mechanism that allows translation, rotation, and removal of the clamp assembly (350, 400) and the viewing element (310) with respect to the cannula (20). The cannula (20) may also be engaged to a flexible arm (160) that is securely mounted in order to stabilize the position of the cannula (20) at the surgical site.

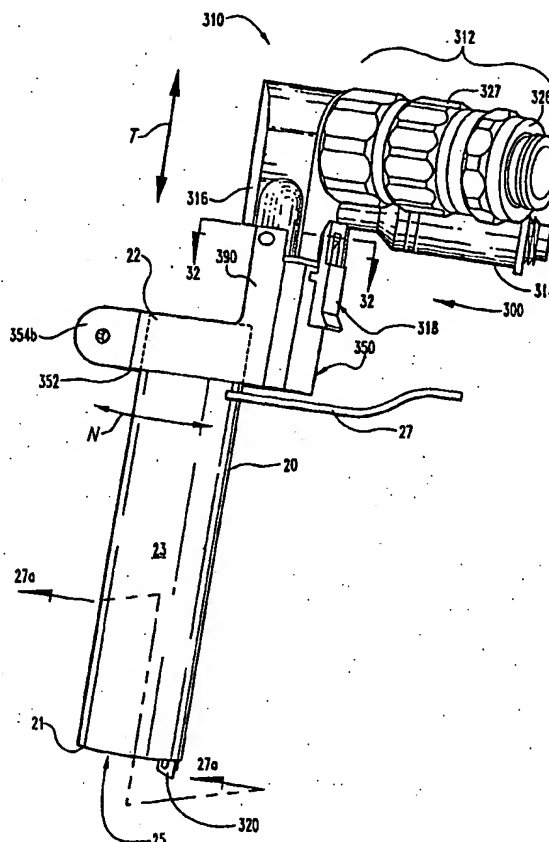

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakhstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LJ	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

DEVICES AND METHODS FOR PERCUTANEOUS SURGERY

RELATED APPLICATIONS

5

This application is a continuation-in-part of U.S. Patent No. 5,902,231 issued May 11, 1999, which is a continuation in part of U.S. Patent No. 5,792,044, each entitled "Devices and Methods for Percutaneous Surgery."

10

BACKGROUND OF THE INVENTION

The present invention relates to devices, instruments and methods for performing percutaneous surgeries, particularly at locations deep within the body. One specific application of the invention concern devices, instruments and techniques for percutaneous, minimally invasive spinal surgery. In another aspect of the invention, the percutaneous surgery is performed under direct vision at any location in the body.

Traditional surgical procedures for pathologies located deep within the body can cause significant trauma to the intervening tissues. These open procedures often require a long incision, extensive muscle stripping, prolonged retraction of tissues, denervation and devascularization of tissue. Most of these surgeries require room time of several hours and several weeks of post-operative recovery time due to the use of general anesthesia and the destruction of tissue during the surgical procedure. In some cases, these invasive procedures lead to permanent scarring and pain that can be more severe than the pain leading to the surgical intervention.

Minimally invasive alternatives such as arthroscopic techniques reduce pain, post-operative recovery time and the destruction of healthy tissue. Orthopedic surgical patients have particularly benefited from minimally invasive surgical techniques. The site of pathology is accessed through portals rather than through a significant incision thus preserving the integrity of the intervening tissues. These minimally invasive techniques also often require only local

30

anesthesia. The avoidance of general anesthesia reduces post-operative recovery time and the risk of complications.

Minimally invasive surgical techniques are particularly desirable for spinal and neurosurgical applications because of the need for access to locations deep within the body and the danger of damage to vital intervening tissues. For example, a common open procedure for disc herniation, laminectomy followed by discectomy requires stripping or dissection of the major muscles of the back to expose the spine. In a posterior approach, tissue including spinal nerves and blood vessels around the dural sac, ligaments and muscle must be retracted to clear a channel from the skin to the disc. These procedures normally take at least one-two hours to perform under general anesthesia and require post-operative recovery periods of at least several weeks. In addition to the long recovery time, the destruction of tissue is a major disadvantage of open spinal procedures. This aspect of open procedures is even more invasive when the discectomy is accompanied by fusion of the adjacent vertebrae. Many patients are reluctant to seek surgery as a solution to pain caused by herniated discs and other spinal conditions because of the severe pain sometimes associated with the muscle dissection.

In order to reduce the post-operative recovery time and pain associated with spinal and other procedures, micro-surgical techniques have been developed. For example, in micro-surgical discectomies, the disc is accessed by cutting a channel from the surface of the patient's back to the disc through a small incision. An operating microscope or loupe is used to visualize the surgical field. Small diameter micro-surgical instruments are passed through the small incision and between two laminae and into the disc. The intervening tissues are disrupted less because the incision is smaller. Although these micro-surgical procedures are less invasive, they still involve some of the same complications associated with open procedures, such as injury to the nerve root and dural sac, perineural scar formation, reherniation at the surgical site and instability due to excess bone removal.

Other attempts have been made for minimally invasive procedures to correct symptomatic spinal conditions. One example is chemonucleolysis which involved the injection of an enzyme into the disc to partially dissolve the nucleus to alleviate disc herniation. Unfortunately, the enzyme, chymopapain, has been
5 plagued by concerns about both its effectiveness and complications such as severe spasms, post-operative pain and sensitivity reactions including anaphylactic shock.

The development of percutaneous spinal procedures has yielded a major improvement in reducing recovery time and post-operative pain because they require minimal, if any, muscle dissection and they can be performed under local
10 anesthesia. For example, U.S. Patent No. 4,545,374 to Jacobson discloses a percutaneous lumbar discectomy using a lateral approach, preferably under fluoroscopic X-ray. This procedure is limited because it does not provide direct visualization of the discectomy site.

Other procedures have been developed which include arthroscopic
15 visualization of the spine and intervening structure. U.S. Patent Nos. 4,573,448 and 5,395,317 to Kambin disclose percutaneous decompression of herniated discs with a posterolateral approach. Fragments of the herniated disc are evacuated through a cannula positioning against the annulus. The '317 Kambin patent discloses a biportal procedure which involves percutaneously placing both a
20 working cannula and a visualization cannula for an endoscope. This procedure allows simultaneous visualization and suction, irrigation and resection in disc procedures.

Unfortunately, disadvantages remain with these procedures and accompanying tools because they are limited to a specific application or approach.
25 For example, Jacobson, Kambin, and other references require a lateral or a posterolateral approach for percutaneous discectomy. These approaches seek to avoid damage to soft tissue structures and the need for bone removal because it was thought to be impractical to cut and remove bone through a channel. However, these approaches do not address other spinal conditions which may
30 require a mid-line approach, removal of bone, or implants.

U.S. Patent No. 5,439,464 to Shapiro discloses a method and instruments for performing arthroscopic spinal surgeries such as laminectomies and fusions with a mid-line or medial posterior approach using three cannulae. Each of the cannulae requires a separate incision. While Shapiro discloses an improvement
5 over prior procedures which were limited to a posterolateral or lateral approach for disc work, Shapiro's procedure still suffers from many of the disadvantages of known prior percutaneous spinal surgery techniques and tools. One disadvantage of the Shapiro procedure is its requirement of a fluid work space. Another significant detriment is that the procedure requires multiple portals into the patient.

10 Fluid is required in these prior procedures to maintain the working space for proper function of optics fixed within a prior art cannula and inserted percutaneously. Irrigation, or the introduction of fluid into the working space, can often be logistically disadvantageous and even dangerous to the patient for several reasons. The introduction of fluid into the working space makes hemostasis more
15 difficult and may damage surrounding tissue. Excess fluid may dangerously dilute the sodium concentration of the patient's blood supply which can cause seizures or worse. The fluid environment can also make drilling difficult due to cavitation. The requirement for a fluid environment generally increases expenses associated with the surgery and adds to the complexity of the surgery, due in part to the
20 relatively high volume of fluid required.

A need has remained for devices and methods that provide for percutaneous minimally invasive surgery for all applications and approaches. A need has also remained for percutaneous methods and devices which do not require a fluid-filled working space, but that can be adapted to a fluid environment if necessary.

25 A significant need is present in this field for techniques and instruments that permit surgical procedures in the working space under direct vision. Procedures that reduce the number of entries into the patient are also highly desirable. The fields of spinal and neuro surgery particularly require devices and techniques that minimize the invasion into the patient and that are streamlined and
30 concise in their application.

SUMMARY OF THE INVENTION

Briefly describing one aspect of the invention, there is provided devices and methods for performing percutaneous procedures under direct visualization, even at locations deep within a patient. In one embodiment, a device for use in percutaneous surgery includes an elongated cannula having a first inner dimensions and an outer dimension sized for percutaneous introduction into a patient. The cannula further includes a distal working end and an opposite proximal end and defines a working channel between the ends having a second dimension which is equal to the first inner dimension. The working channel is sized to receive a tool therethrough. The device also includes a viewing element mounted inside the cannula adjacent the working channel. The viewing element has a first end connectable to a viewing apparatus and an opposite second end disposed adjacent the distal working end of the cannula. In some embodiments, the viewing element can be a fiber optic cable, a GRIN rod, a rod-lens device or a remote optics ("chip on a stick") device.

In another aspect, a fixture is provided for mounting the viewing element to the cannula. The fixture includes a housing attachable to the proximal end of the cannula. The housing defines a working channel opening therethrough in communication with the working channel. The working channel opening is sized to substantially correspond to the second dimension of the working channel. The housing also defines an optics bore adjacent the working channel opening. The optics bore is sized to receive the elongated viewing element therethrough.

In some embodiments, the fixture supports the viewing device for movement within the optics bore along the longitudinal axis of the bore to extend or retract the lens relative to the distal working end of the cannula. In other embodiments, the fixture supports the viewing device for rotation within the optics bore about the longitudinal axis of the bore. In some embodiments, the housing is rotatable relative to the cannula so that the longitudinal axis of the optics bore is rotatable about the longitudinal axis of the working channel.

In one aspect of the invention, the working channel can be created by components other than a tubular cannula. For example, an expanding tissue dilator

or tissue retractor is also contemplated. With this modification, the fixture would engage the dilator or retractor in its expanded condition.

In a further aspect of the invention, the optical viewing device is connected to a tissue retractor, such as a speculum. An apparatus of this type can be particularly useful in various applications such as transnasal transphenoidal surgery and pituitary procedures.

In accordance with one embodiment, the fixture includes at least one irrigation/aspiration port. Preferably, the port(s) can communicate with at least one irrigation/aspiration channel in the optical viewing device. In this manner, irrigation and/or aspiration can also be applied at the surgical site. When aspiration alone is applied, the port is connected to a vacuum or suction source. The aspiration will draw ambient air through the working channel, across the distal working space, and into the irrigation/aspiration channel of the viewing device. One benefit is that this ambient air aspiration eliminates smoke generated by various working tools and clears the optics lens of fog and debris.

In another embodiment, the fixture can be supported adjacent the proximal end of the cannula by a clamp engaging the outer surface of the cannula. In one specific embodiment, the clamp is a barrel clamp mechanism that is selectively operated by a lever arm and barrel cam. With this embodiment, the fixture itself can be translated along the length of the cannula to extend or retract the lens of the viewing device relative to the end of the working channel.

According to the methods of this invention, spinal and other surgeries can be performed percutaneously with direct visualization. In another aspect of the inventive surgical techniques, all steps of a surgical procedure are conducted under direct vision through a single working channel cannula. An optical scope or viewing device is moved within the working channel and throughout the working space from a variety of angles and orientations to provide a clear view of the operative steps. The techniques of the present invention also encompass passing multiple tools and instruments through the single working channel cannula and manipulating the instruments and tools within the working space.

In another embodiment of the present invention, a clamp assembly is movably engaged to the outer surface of the cannula and a viewing element releasably engaged to said clamp assembly. The clamp assembly includes a viewing element receiving portion releasably engaged to a clamp assembly engaging portion of the viewing element. The receiving portion defines a receptacle and the engaging portion includes a dovetail configured to be slidingly received within the receptacle.

In yet another embodiment of the present invention, an assembly for supporting a viewing element adjacent a cannula includes a ring having a pair of free ends and sized to substantially encircle the cannula. A mechanism engaged to the ring biases the free ends towards one another to engage the outer surface of the cannula. A viewing element receiving portion extends from the ring.

In accordance with one aspect of the invention, the ring includes a first arm pivotably coupled to a second arm, each of the arms having a free end adjacent the other free end. The mechanism includes a lever arm extending from each of the arms, and a hinge pivotably couples and biases the first and second arms against the outer surface of the cannula.

In another aspect of the invention, the ring includes a pair of opposing arms extending from a corresponding one of the free ends. The arms define a slot extending between the free ends and the mechanism is operable to compress the arms together. In a further aspect, one of the arms includes at least one projection extending therefrom. The mechanism has a lever arm with an inside face facing the at least one projection, the inside face including a cam surface with at least one inclined ramp. A fastener rotatably engages the lever arm to the pair of arms with the cam surface disposed for contact with the at least one projection. Rotation of the lever arm relative to the pair of arms causes the at least one projection to slide along the ramp to push the pair of arms toward each other to narrow the slot.

It is an object of the invention to provide devices and methods for percutaneous spinal surgery for all applications and approaches. One advantage of this invention is that multiple percutaneous procedures can be accomplished via a single viewing element because the viewing element is usable with clamp

assemblies that engage various shaped and sized cannulas. One benefit of this invention is that it provides instruments and methods which reduce the cost, risk, pain and recovery time associated with surgery. These and other objects, advantages and features are accomplished according to the devices and methods of

5 the present invention.

DESCRIPTION OF THE FIGURES

FIG. 1 is a side elevational view of a device according to this invention.

FIG. 2 is a top elevational view of a fixture for supporting a viewing device
5 within a cannula according to this invention.

FIG. 3 is a side cross-sectional view of the fixture shown in FIG. 2.

FIG. 4 is a side elevational view of a retractor according to one
embodiment of this invention.

FIG. 4A is an end cross-sectional view of the retractor of FIG. 4 taken
10 along lines A-A.

FIG. 5 is a top elevational view of the retractor shown in FIG. 4.

FIG. 6 is an end elevational view of the retractor shown in FIGS. 4 and 5.

FIG. 7 is a side elevational view of a retractor according to another
embodiment of this invention.

FIG. 7A is an end cross-sectional view of the retractor of FIG. 7 taken
15 along lines A-A.

FIG. 7B is an end cross-sectional view of the retractor of FIG. 7 taken
along lines B-B.

FIG. 8 is a top elevational view of the retractor shown in FIG. 7.

FIG. 9 is a side elevational view of a dilator according to this invention.
20

FIG. 10 (a) –(i) depicts the steps of a method according to this invention.

FIG. 11 is a side cross-sectional view of a device according to one
embodiment of this invention.

FIG. 12 is a side cross-sectional view of an aspiration cap as shown in FIG.
25 11.

FIG. 13 is a top perspective view of a device according to another
embodiment of the present invention.

FIG. 14 is a side perspective view of a fixture for supporting a viewing
device forming part of the device shown in FIG. 13.

FIG. 15 is a side elevational view of the device depicted in FIG. 13 with the
30 device shown connected to optical equipment depicted in phantom lines.

FIG. 16 is a side elevational view of a scope body forming part of the fixture depicted in FIGS. 13 and 14.

FIG. 17 is a bottom elevational view of the scope body shown in FIG. 16.

FIG. 18 is a top elevational view of a lever arm forming part of a barrel clamp mechanism used with the fixture depicted in FIG. 14.

FIG. 19 is an end cross-sectional view of the lever arm shown in FIG. 18 taken along line 19-19 as viewed in the direction of the arrows.

FIG. 20 is a top elevational view of a barrel cam forming part of a barrel clamp mechanism incorporated into the fixture depicted in FIG. 14.

FIG. 21 is a side elevational view of the barrel cam shown in FIG. 20.

FIG. 22 is a bottom assembly view showing the assembly of the lever arm of FIGS. 18-19, the barrel cam of FIGS. 20-21 with the scope body shown in FIG. 14.

FIG. 23 is a side elevational view of a scope body as depicted in FIG. 14 connected to an aspiration circuit.

FIG. 24 is a cross-sectional view of a human patient at a lumbar vertebral level with a device according to one embodiment of the invention situated within the patient to define a working channel above the laminae of the vertebra.

FIG. 25 is a side elevational view of a tissue retractor incorporating an optical viewing device.

FIG. 26 is a top elevational view of the tissue retractor incorporating an optical viewing device as shown in FIG. 25.

FIG. 27 is a side perspective view of a device according to another embodiment of the present invention.

FIG. 27a is a section view along line 27a-27a of FIG. 27.

FIG. 28 is a side perspective view of a modular clamp and endoscope assembly forming part of the device of FIG. 27.

FIG. 29 is a side perspective view of one embodiment of a modular clamp for use with the assembly of FIG. 28.

FIG. 30 is a side perspective view of one embodiment of an endoscope for use with the assembly of FIG. 29.

FIG. 31 is a side elevational view of a coupling mechanism forming a part of the assembly of FIG. 28.

FIG. 32 is a partially fragmented cross-sectional view of the device taken along line 32-32 of FIG. 27.

5 FIG. 33 is a perspective view of one embodiment of a lever arm forming part of the barrel clamp mechanism shown in FIG. 32.

FIG. 34 is a perspective view of another embodiment of a lever arm forming part of the barrel clamp mechanism of FIG. 32.

10 FIG. 35 is a partially fragmented cross-sectional view of an alternate embodiment of the device illustrated in FIG. 32.

FIG. 36 is a sectional view of an alternate embodiment cross-section of a cannula for use with the present invention.

FIG. 37 is a sectional view of another alternate embodiment cross-section of a cannula for use with the present invention.

DESCRIPTION OF THE PREFERRED EMBODIMENTS

For the purposes of promoting an understanding of the principles of the invention, reference will now be made to the embodiments illustrated in the drawings and specific language will be used to describe the same. It will
5 nevertheless be understood that no limitation of the scope of the invention is thereby intended, such alterations and further modifications in the illustrated devices and described methods, and such further applications of the principles of the invention as illustrated therein being contemplated as would normally occur to
10 one skilled in the art to which the invention relates.

The present invention provides instruments and methods for performing percutaneous surgery, including spinal applications such as laminotomy, laminectomy, foramenotomy, facetectomy or discectomy, with a single working
channel endoscope. The present inventors have discovered that many
15 percutaneous surgeries may be performed without a fluid workspace through the use of optics which move independently of the cannula. The present invention contemplates techniques and instruments that can be implemented with or without a fluid environment.

This invention also brings the advantages of percutaneous procedures to
20 applications that previously required open surgery. One advantage is based upon the further discovery that bone work can be performed percutaneously through a large working channel. Another advantage is realized in the use of a single portal within the patient to perform a wide range of simultaneous procedures.

According to one embodiment of the present invention, as depicted in FIG.
25 1, a device 10 is provided for use in percutaneous surgery which includes an elongated cannula 20 having a first inner diameter D_1 and an outer diameter D_0 sized for percutaneous introduction into a patient. The cannula 20 also includes a distal working end 21 and an opposite proximal end 22. The cannula defines a working channel 25 between the ends 21, 22 having a second diameter d_2 equal to
30 the first inner diameter D_1 sized for receiving a tool therethrough. The cannula has a length along its longitudinal axis L that is sized to pass through the patient from

the skin to an operative site or working space. In some cases, the working space may be adjacent a vertebra or disc, or in the spinal canal.

An elongated viewing element 50 is mountable inside cannula 20 adjacent the working channel 25. The viewing element 50 has a first end 51 connectable to a viewing apparatus, such as an eyepiece or camera, and an opposite second end 52 disposed or positionable adjacent the distal working end 21 of the cannula 20. The particular elongated viewing element 50 is not critical to the invention. Any suitable viewing element is contemplated that creates an optical or image transmission channel. In one embodiment, the elongated viewing element 50 includes a fiber optic scope 54 and a lens 55 at the second end 52. Preferably, the fiber optic scope includes illumination fibers and image transmission fibers (not shown). Alternatively, the viewing element may be a rigid endoscope or an endoscope having a steerable or bendable tip.

One advantage of this invention is that it provides optics which are movable relative to the cannula 20. Because the optics are movable, it is not necessary to provide a fluid-maintained work space. The optics can be removed, cleaned and replaced while the cannula is percutaneously positioned within the patient over the working space. Any configuration which allows the optics to be movably supported adjacent the working channel 25 is contemplated. In one embodiment, shown in FIGS. 1-3, a fixture 30 is provided for mounting the elongated viewing element 50 to the cannula 20. Preferably, the fixture 30 includes a housing 31 attachable to the proximal end 22 of the cannula 20. The working channel opening 35 is sized to substantially correspond to the second diameter d_2 of the working channel 25 to receive tools. The fixture 30 includes a housing 31 which defines a working channel opening 35 arranged to communicate with the working channel 25 when the fixture 30 is mounted to the cannula 20. The working channel opening 35 is sized to receive tools therethrough for passage through the working channel 25. In the embodiments shown in FIGS. 1-3, the fixture 30 is configured to mount the viewing element 50 within the working channel 25.

The housing 31 also defines an optics bore 60 adjacent the working channel opening 35. The optics bore 60 has a longitudinal axis ℓ that is preferably substantially parallel to the axis L of the cannula and working channel. The optics bore 60 is preferably sized to removably receive the elongated viewing element 50 therethrough. The fixture 30 preferably supports the viewing element 50 for movement within the optics bore 60 along the longitudinal axis ℓ of the bore 60 to extend or retract the lens 55 relative to the distal working end 21 of the cannula 20. The retractable/extendable feature of the optics of this invention provides an advantage over prior endoscopes because it eliminates the requirement for a fluid workspace. While the device 10 and its viewing element 50 can be easily used in a fluid environment, the fluid is not essential for the system to operate, contrary to prior systems. Furthermore, many of the prior endoscopes were not suited to access certain areas because of their large diameters. For example, prior endoscopes could not access the spinal canal. However, with this invention, access to the spinal canal is not limited by the diameter of the channel or cannula. The cannula 20 can be left behind in the soft tissue or supported by the lamina while the second end 52 of the elongated viewing element 50 can be advanced into the spinal canal along with any spinal instruments which have been inserted into the working channel 25.

Preferably the fixture 30 also supports the viewing element 50 for the rotation within the optics bore 60 about the longitudinal axis ℓ of the bore 60. The lens 55 of the viewing element 50 defines an optical axis A_0 . As in many endoscopes, the optical axis A_0 can be offset at an angle relative to the longitudinal axis ℓ of the optics bore 60. This feature allows the optical axis A_0 of the lens to be swept through a conical field of the view F for greater visibility of the working space. The fixture 30 can further be configured so that the viewing element 50 is rotatable relative to the cannula 20. In this embodiment, the housing 31 is rotatable relative to the cannula 20 so that the second longitudinal axis ℓ of the optics bore 60 rotates about the longitudinal axis L of the working channel 25. The

rotatable features of this invention allows visualization of the entire working space. This feature also aids in simplifying the surgical procedure because the optics 50 and accompanying fittings can be moved out of the way of the surgeon's hands and tools passing through the working channel.

5 In one embodiment depicted in FIG. 3, the housing 31 defines a receiver bore 40 having an inner diameter d_i slightly larger than the outer diameter D_o of the cannula 20. In this configuration, the proximal end 22 of the cannula 20 can be received within the receiver bore 40 so that the housing 31 can rotate about the proximal end 22 of the cannula 20. As shown in FIG. 3, the housing 31 also
10 includes an upper bore 41 which is contiguous with the working channel opening 35 and the receiver bore 40. In one embodiment, the optics bore 60 is disposed within the upper bore 41 of the housing 31.

In a preferred embodiment depicted in FIG. 2, the optics bore 60 is defined by a C-shaped clip 61 disposed within the upper bore 41. Preferably, the C-shaped
15 clip 61 is formed of a resilient material and the optics bore 60 defined by the clip 61 has an inner diameter D_i that is slightly less than the outer diameter of the elongated viewing element 50. When the viewing element 50 is pushed into the optics bore 60 it resiliently deflects the C-shaped clip 61. The resilience of the clip 61 provides a gripping force on the element 50 to hold it in the desired position,
20 while still allowing the element 50 to be repositioned. Alternatively, the optics bore 60 can have an inner diameter larger than the outer diameter of the viewing element. In this instance, the viewing element 50 can be supported outside the device 20, either manually or by a separate support fixture.

Preferably the device 10 provides engagement means for securely yet
25 rotatably engaging the fixture 30 to the cannula 20. Most preferably, the fixture 30 is configured to engage a standard cannula 20. Engagement means can be disposed between the housing 31 and the cannula 20 when the fixture 30 is mounted to the proximal end 22 of the cannula 20 for providing gripping engagement between the housing 31 and the cannula 20. In one embodiment
30 depicted in FIG. 3 the engagement means includes a number of grooves 32 within the receiver bore 40 and a resilient sealing member, such as an O-ring (see FIG.

11) disposed in each groove 32. The sealing members, or O-rings, disposed between the housing 31 and the outer diameter D_0 of the cannula 20 rotatably secure the fixture 30 to the cannula 20. The O-rings provide sufficient resistance to movement to hold the fixture 30 in a selected position on the cannula. In
5 another embodiment, the housing 31 defines a receiver bore 40 which has an inner diameter d_1 which is only slightly larger than the outer diameter D_0 of the cannula 20 so that the housing 31 can rotate freely about the cannula 20.

The working channel 25 and the working channel opening 35 are both sized to receive a tool or instrument therethrough. Preferably, the working channel
10 opening 35 of the housing 31 has a diameter D_w which is substantially equal to the inner diameter d_2 of the working channel 25 so that the effective diameter of the working channel is not reduced by the fixture 30. This configuration provides a maximum amount of space for the insertion of tools into the working channel 25. The present invention is advantageous because standard micro-surgical spinal tools
15 can be inserted into the working channel and manipulated to perform a surgical procedure. The present invention is particularly advantageous because the working channel 25 will simultaneously accept a plurality of movable instruments. No other known prior art device has a working channel that accepts more than one movable instrument at a time through a single port. Therefore, according to this
20 invention, an entire percutaneous surgical procedure can be performed through the working channel 25 of the device 10 under direct visualization using the viewing element 50 disposed within the optics bore 60.

In accordance with the present embodiment, the components of the device 10 are cylindrical in configuration. In other words, the cannula 20, working
25 channel 25 and fixture 30 have corresponding cylindrical configurations which yield the various diameters D_i , D_o , D_w and d_2 . In accordance with other embodiments contemplated as part of the invention, these diameters may be non-circular inner and outer dimensions, such as oval or square shaped. For example, a cannula 20 modified to a square cross-section, such as illustrated in FIG.37, would
30 still provide a large working channel, such as working channel 25. In another embodiment, the cross-section is oval, such as that illustrated in FIG. 36.

Likewise, a corresponding fixture 30 have a square cross-section would also provide a large working channel opening D_w . In the case of the non-circular configurations, the fixture 30 in accordance with the present embodiment would be unable to rotate around the circumference of the cannula 20, as permitted by the circular configurations. On the other hand, even the non-circular configurations will permit axial movement of the optical viewing element and rotation of the viewing element about its own axis, as set forth more fully herein.

In accordance with a further variation of the present invention, the cannula 20 can be replaced by a similar device that is capable of maintaining a large working channel 25. For example, the cannula 20 can be replaced by an expanding cannula or dilator apparatus. In one specific embodiment, the apparatus can be a spiral wound tube that is unwound or expanded to provide the working channel dimension. Alternatively, multiple tissue dilators, such as speculae, can be expanded to create a working space. In these configurations, the fixture 30 may still be used to support the optical viewing element 50 once the expandable dilator or tissue retractor reaches its full working channel dimension.

Although standard micro-surgical instruments may be used with the present invention, this invention also contemplates certain novel tools which capitalize on and enhance the advantages of this invention.

According to one preferred embodiment of the invention, a tissue retractor 70 is provided as depicted in FIGS. 4-6. The retractor 70 is removably and rotatably insertable through the working channel 25 and the working channel opening 35 of the device 10. The tissue retractor 70 includes a working tip 75 configured to atraumatically displace tissue as the retractor 70 is manipulated through the tissue and a body 76 having a proximal first end 77 and a distal second end 78. The second end 78 can be integral with the working tip 75 which preferably has a blunt curved end 82. In addition, the working tip 75 is also preferably bent or curved away from the body 76, as shown in FIG. 4. The body 76 is sized to be rotatably received within the cannula 20 and has a length B from the first end 77 to the second end 78 sufficient so that the first end 77 and the

working tip 75 can both extend outside the cannula 20 when the body 76 is within the cannula 20.

This invention contemplates any suitable retractor for use through the working channel 25. However, retractors such as the retractor 70 depicted in
5 FIGS. 4-6 are preferred in which the body 76 includes a curved plate 84 that is configured to conform to the inner cylindrical surface 26 of the cannula without substantially blocking the working channel 25. The curved plate 84 has a convex surface 80 and an opposite concave surface 81. In one embodiment, the curved plate 84 includes a first plate portion 85 defining a first convex surface 80 and an
10 opposite first concave surface 81. A second plate portion 86 is integral with the first plate portion 85 and is disposed between the first plate portion 85 and the working tip 75. The second plate portion 86 defines a second convex surface (not shown) and an opposite second concave surface 81'. Both the first plate portion 85 and the second plate portion 86 include opposite edges 90 extending substantially
15 parallel to the length B of the body 76.

Preferably, the curved plate 84 subtends an arc A_1 between the opposite edges 90 of at least 200 degrees, and most preferably 270 degrees. In a specific embodiment, the second plate portion 86 and specifically the second concave surface 81' subtends an angle that decreases along the length of the retractor.
20 Thus, in one embodiment, the second concave surface 81' subtends an angle of about 200 degrees adjacent the first plate portion 85, decreasing to an angle of less than about 10 degrees at end 78.

An alternate embodiment of a tissue retractor according to this invention is depicted in FIGS. 7-8. This retractor 100 has a body 106 which includes a first
25 plate portion 115 defining a first convex surface 110 and an opposite first concave surface 111 and includes first opposite edges 120 extending substantially parallel to the length B of the body 106. The first plate portion 115 subtends a first arc A_2 between the first opposite edges 120. The retractor body 106 also includes a second plate portion 116 which is integral with the first plate portion 115 and is
30 disposed between the first plate portion 115 and a working tip 105. The second plate portion 116 defines a second convex surface 110' and an opposite second

concave surface 111' and includes second opposite edges 120' extending substantially parallel to the length B. The second plate portion 116 subtends a second arc A_3 between the second opposite edges 120' that is different from the first arc A_2 in this embodiment. Preferably, the first arc A_2 subtends an angle of less than 180 degrees and the second arc A_3 subtends an angle of more than 180 degrees. Most preferably, the first arc A_2 subtends an angle of about 90 degrees and the second arc A_3 subtends an angle of about 270 degrees.

The retractors of this invention may be provided with means for engaging the retractors 70, 100 within the working channel 25 of the cannula 20. For example, the convex surfaces 80, 110 can be configured to have a diameter that is greater than the diameter D_1 of the inner cylindrical surface 26 of the cannula 20. In that case, the body 76, 106 may be formed of a resilient material that is deformable to be insertable into the cannula 20 so that the convex surface 80, 110 is in contact with the inner cylindrical surface 26 of the cannula 20. When the body 76, 106 is deformed, it exerts an outward force against the surface 26 to frictionally hold the retractor in its selected position.

The preferred components provided by this invention are configured so that multiple tools and instruments can be accepted and manipulated within the working channel 25 of the cannula 20. The components are also configured so that more than one surgeon may manipulate instruments through the working channel 25 of the cannula 20 at one time. For example, one surgeon may be manipulating the retractor while another surgeon is drilling into a bone. The curvature of the body 76, 106 of the retractors 70, 100 provides more working space and increases visibility. Another feature is that the long axis of the component can be placed in the working channel 25 while a bend in the handle portion keeps hands away from the channel 25 so that more than one surgeon can work in the channel 25 and more tools can be placed in the channel 25. The retractors shown in FIGS. 4-8 each comprise an arm 71, 101 attached to the proximal first end 77, 107 of the body 76, 106. Preferably, as shown in FIGS. 4-8, the arm 71, 101 is at an angle α is about 90 degrees so that the arm 71, 101 is substantially perpendicular to the length L of

the body 76, 106. Preferably, the arm 71, 101 has a gripping surface 72, 102 to facilitate manipulation of the retractor 70, 100.

The present invention also provides tissue dilators usable with the device 10. Any dilator which is insertable into the working channel 25 of the cannula 20 is contemplated; however, a s preferred dilator provided by this invention is depicted in FIG. 9. A dilator 130 preferably includes a hollow sleeve 135 defining a channel 131. The channel 131 allows the dilator 130 to be placed over a guidewire (not shown) or other dilators. The hollow sleeve 135 has a working end 136 defining a first opening 132 in communication with the channel 131 and an opposite end 137 defining a second opening 133. The working end 136 is tapered to a tapered tip 138 to atraumatically displace tissue. Preferably, a gripping portion 140 is provided on the outer surface 141 of the sleeve 135 adjacent the opposite end 137. In one embodiment, the gripping portion 140 is defined by a plurality of circumferential grooves 142 defined in the outer surface 141. The grooves 142 are configured for manual gripping of the dilator 130 to manipulate the dilator 130 through tissue. Preferably, the grooves 142 are partially cylindrical. In the embodiment shown in FIG. 9, the gripping portion 140 includes a number of circumferential flats 143 adjacent each of the circumferential grooves 142. The grooves 142 have a first width W_1 along the length of the sleeve 135 and the flats 143 have a second width W_2 along the length. Preferably, the first and second width W_1 and W_2 are substantially equal.

The present invention has application to a wide range of surgical procedures, and particularly spinal procedures such as laminotomy, laminectomy, foramenotomy, facetectomy and discectomy. Prior surgical techniques for each of these procedures has evolved from a grossly invasive open surgeries to the minimally invasive techniques represented by the patents of Kambin and Shapiro. However, in each of these minimally invasive techniques, multiple entries into the patent is required. Moreover, most of the prior minimally invasive techniques are readily adapted only for a posterolateral approach to the spine. The devices and instruments of present invention have application in an inventive surgical technique that permits each of these several types of surgical procedures to be

performed via a single working channel. This invention can also be used from any approach and in other regions besides the spine. For instance, the invention contemplates apparatus appropriately sized for use in transnasal, transphenoidal and pituitary surgeries.

5 The steps of the spinal surgical procedure in accordance with one aspect of the present invention are depicted in FIG. 10. As can be readily seen from each of the depicted steps (a)-(i), the present embodiment of the invention permits a substantially mid-line or medial posterior approach to the spine. Of course, it is understood that many of the following surgical steps can be performed from other
10 approaches to the spine, such as posterolateral and anterior. In a first step of the technique, a guidewire 150 can be advanced through the skin and tissue into the laminae M of a vertebral body V. Preferably, a small incision is made in the skin to facilitate penetration of the guidewire through the skin. In addition, most preferably the guidewire, which may be a K-wire, is inserted under radiographic or
15 image guided control to verify its proper positioning within the laminae M of the vertebra V. It is, of course, understood that the guidewire 150 can be positioned at virtually any location in the spine and in any portion of a vertebra V. The positioning of the guidewire is dependent upon the surgical procedure to be conducted through the working channel cannula of the present invention.
20 Preferably, the guidewire 150 is solidly anchored into the vertebral bone, being tapped by a mallet if necessary.

 In subsequent steps of the preferred method, a series of tissue dilators are advanced over the guidewire 150, as depicted in steps (b)-(d) in FIG. 10. Alternatively, the dilators can be advanced through the incision without the aid of a
25 guidewire, followed by blunt dissection of the underlying tissues. In the specific illustrated embodiment, a series of successively larger dilators 151, 152 and 153 are concentrically disposed over each other and over the guidewire 150 and advanced into the body to sequentially dilate the perispinous soft tissues. Most preferably, the tissue dilators are of the type shown in FIG. 9 of the present
30 application. In a specific embodiment, the dilators have successively larger diameters, ranging from 5mm, to 9mm to 12.5mm for the largest dilator. Other

dilator sizes are contemplated depending upon the anatomical approach and upon the desired size of the working channel.

In the next step of the illustrated technique, the working channel cannula 20 is advanced over the largest dilator 153, as shown in step (e), and the dilators and guidewire 150 are removed, as shown in step (f). Preferably, the working channel cannula 20 has an inner diameter D_1 of 12.7mm so that it can be easily advanced over the 12.5mm outer diameter of the large dilator 153. Larger working channel cannulas are contemplated depending upon the anatomical region and surgical procedure.

With the cannula 20 in position, a working channel is formed between the skin of the patient to a working space adjacent the spine. It is understood that the length of the cannula 20 is determined by the particular surgical operation being performed and the anatomy surrounding the working space. For instance, in the lumbar spine the distance between the laminae M of a vertebra V to the skin of the patient requires a longer cannula 20 than a similar procedure performed in the cervical spine where the vertebral body is closer to the skin. In one specific embodiment in which the cannula 20 is used in a lumbar discectomy procedure, the cannula has a length of 87mm, although generally only about half of the length of the cannula will be situated within the patient during the procedure.

In accordance with the present surgical technique, the working channel cannula 20 is at least initially only supported by the soft tissue and skin of the patient. Thus, in one aspect of the preferred embodiment, the cannula 20 can include a mounting bracket 27 affixed to the outer surface of the cannula (FIG. 10(f), FIG. 11). This mounting bracket 27 can be fastened to a flexible support arm 160, which can be of known design. Preferably, the flexible support arm 160 is engaged to the bracket 27 by way of a bolt and wing nut 161, as shown in FIG. 10(i) and in more detail in FIG. 11, although other fasteners are also contemplated. This flexible arm 160 can be mounted to the surgical table and can be readily adjusted into a fixed position to provide firm support for the cannula 20. The flexible arm 160 is preferred so that it can be contoured as required to stay clear of

the surgical site and to allow the surgeons adequate room to manipulate the variety of tools that would be used throughout the procedure.

Returning to FIG. 10, once the cannula 20 is seated within the patient, the fixture 30 can be engaged over the proximal end of the cannula 20. The fixture 30, as shown in FIGS. 2 and 3 and as described above, provides an optics bore 60 for supporting an elongated viewing element, such as element 50 shown in step h. In accordance with the invention, the viewing element 50 is advanced into the fixture 30 and supported by the optics bore 60 (FIG. 2). In one specific embodiment, the element 50 is most preferably a fiber optic scope, although a rod lens scope, "chip on a stick" or other viewing scopes may be utilized. In the final step (i) of the procedure shown in FIG. 10, the flexible arm 160 is mounted to the bracket 27 to support the cannula 20 which in turn supports the optical viewing element 50. This final position of step (i) in FIG. 10 is shown in more detail in FIG. 11. The viewing element 50 can be a variety of types, including a rigid endoscope or a flexible and steerable scope.

With the viewing element or scope 50 supported by the fixture 30 the surgeon can directly visualize the area beneath the working channel 25 of the cannula 20. The surgeon can freely manipulate the viewing element 50 within the working channel 25 or beyond the distal end of the cannula into the working space. In the case of a steerable tip scope, the second end 52 of the viewing element 50, which carries the lens 55, can be manipulated to different positions, such as shown in FIG. 11. With virtually any type of viewing element, the manipulation and positioning of the scope is not limited by the procedure to be performed. For instance, in the case of a laminotomy, laminectomy, foramenotomy or facetectomy, a variety of rongeurs, curettes, and trephines can be extended through the working channel opening 35 (see FIG. 2) and through the working channel 25 of the cannula 20 (see FIG. 11) into the working space. It is understood that these various tools and instruments are designed to fit through the working channel. For instance, in one specific embodiment, the working channel 25 through the cannula 20 can have a maximum diameter d_2 of 12.7mm. However, with the viewing element 50 extending into the working channel 25, the effective diameter is about

8mm in the specific illustrated embodiment, although adequate space is provided within the working channel 25 around the viewing element 50 to allow a wide range of movement of the tool or instrument within the working channel. The present invention is not limited to particular sizes for the working channel and
5 effective diameter, since the dimensions of the components will depend upon the anatomy of the surgical site and the type of procedure being performed.

Preferably, each of the tools and instruments used with the working channel cannula 20 are designed to minimize obstruction of the surgeon's visualization of and access to the working space at the distal end of the working channel cannula.
10 Likewise, the instruments and tools are designed so that their actuating ends which are manipulated by the surgeon are displaced from the working channel cannula 20. One such example is the tissue retractor shown in FIGS. 4-8. With these retractors, the handles that are manually gripped by the surgeon are offset at about a 90 degree angle relative to the longitudinal axis of the tool itself.

15 In accordance with once aspect of the present invention, the surgical procedures conducted through the working channel cannula 20 and within the working space at the distal end of the cannula are performed "dry" – that is, without the use of irrigation fluid. In prior surgical techniques, the working space at the surgical site is fluid filled to maintain the working space and to assist in the
20 use of the visualization optics. However, in these prior systems the visualization optics were fixed within the endoscope. In contrast, the device 10 of the present invention allows a wide range of movement for the viewing element 50 so that the lens 55 can be retracted completely within the working channel 25 of the cannula 20 to protect it from contact with the perispinous tissue or blood that may be
25 generated at the surgical site.

Moreover, since the viewing element 50 is removable and replaceable, the element 50 can be completely removed from the fixture 30 so that the lens 55 can be cleaned, after which the viewing element 50 can be reinserted into the fixture and advanced back to the working space. Under these circumstances, then the
30 need for irrigation is less critical. This feature can be of particular value when cutting operations are being performed by a power drill. It has been found in prior

surgical procedures that the use of a power drill in a fluid environment can cause turbulence or cavitation of the fluid. This turbulence can completely shroud the surgeon's view of the surgical site at least while the drill is being operated. With the present invention, the dry environment allows continuous viewing of the operation of the power drill so that the surgeon can quickly and efficiently perform the necessary cutting procedures.

While the present invention permits the surgeon to conduct surgical procedures in the working space under a dry environment, irrigation may be provided separately through the working channel 25. Alternatively, the viewing device 50 itself may include a tube 54 supported by the fitting 53 through which modest amount of fluid can be provided to keep the visualization space clear. In addition, during a discectomy, aspiration of the excised tissue is preferred, and irrigation will frequently assist in rapid removal of this tissue. Thus, separate irrigation and aspiration elements can also be inserted through the working channel 25 as required by the procedure.

As necessary, aspiration can be conducted directly through the working channel 25 of the cannula 20. In one specific embodiment, an aspiration cap 165 is provided as shown in FIGS. 11 and 12. The cap 165 includes a body 166 which defines a mating bore 167 having an inner diameter d_b larger than the outer diameter D_h of the housing 31 of fitting 30. A tool opening 168 is provided in communication with the mating bore 167. When the aspiration cap 165 is mounted over the housing 31, as shown in FIG. 11, the tool opening 168 communicates directly with the upper bore 41 and provides the same entry capabilities as the working channel opening 35 of the housing 31. The aspiration cap 165 is also provided with a tube receiver bore 169 which intersects the mating bore 167. The receiver bore 169 is configured to receive an aspiration tube through which a vacuum or suction is applied. In certain instances, the tool opening 168 may be covered while suction is applied through the tool receiver bore 169 and mating bore 167, and ultimately, through the working channel 25. Covering the opening 168 can optimize the aspiration effect through the working channel.

Returning again to the surgical technique of one embodiment of the present invention, once the working channel cannula 20 and the optics 50 are in position, as depicted in FIG. 10 step (i) and FIG. 11, the paraspinous tissue can be retracted using instruments as described above, and a laminectomy performed using various
5 rongeurs, curettes and drills. As necessary, the cannula 20 can be angled to allow a greater region of bone removal, which may be necessary for access to other portions of the spinal anatomy. In some instances, access to the spinal canal and the posterior medial aspects of the disc annulus may require cutting a portion of the vertebral bone that is greater than the inner diameter of the working channel 25.
10 Thus, some manipulation of the cannula 20 may be necessary to permit removal of a greater portion of bone. In other operations, multi-level laminectomies or foramenotomies may be necessary. In this instance, these multi-level procedures can be conducted by sequentially inserting the working channel cannula 20 through several small cutaneous incisions along the spinal mid-line. Alternatively, several
15 working channel cannulas 20 can be placed at each of the small cutaneous incisions to perform the multi-level bone removal procedures.

Again, in accordance with the preferred illustrated surgical technique, an opening is cut into the laminae M of the vertebra V providing direct visual access to the spinal canal itself. As necessary, tissue surrounding the spinal nerve root
20 can be removed utilizing micro-surgical knives and curettes. Once the spinal nerve root is exposed, a retractor, such as the retractors shown in FIGS. 4-8, can be used to gently move and hold the nerve root outside the working space. In one importance aspect of the two retractors 70, 100, the portion of the retractor passing through the working channel 25 generally conforms to the inner surface of the
25 cannula 20 so that the working channel 25 is not disrupted by the retractor tool. Specifically, the effective diameter within the working channel 25 is reduced only by the thickness of the curved plates 84, 114 of the retractors 70, 100. In one specific embodiment, this thickness is about 0.3mm, so it can be seen that the tissue retractors do not significantly reduce the space available in the working
30 channel 25 for insertion of other tools and instruments.

With the tissue retractor in place within the working channel 25, bone within the spinal canal, such as may occur in a burst fracture, can be removed with a curette or a high speed drill. Alternatively, the fractured bone may be impacted back into the vertebral body with a bone impactor. At this point, if the spinal procedure to be performed is the removal of epidural spinal tumors, the tumors can be resected utilizing various micro-surgical instruments. In other procedures, the dura may be opened and the intradural pathology may be approached with micro-surgical instruments passing through the working channel cannula 20. In accordance with the specific illustrated technique, the nerve root retracted posterior medial disc herniations can be readily excised directly at the site of the herniation.

In another embodiment of the invention, a working channel cannula, such as cannula 20, is provided with a fixture 170 for supporting optics and irrigation/aspiration components. In accordance with this embodiment, the fixture 170 includes a scope body 171 which is shown most clearly in FIGS. 13, 14, 16, and 17. The scope body 171 includes a clamping ring 172 configured to encircle the outer surfaces 23 of the cannula 20. In particular, the clamping ring 172 includes an inner clamping surface 175 (see FIG. 14). The clamping surface 175 has substantially the same configuration and dimension as the outer surface 23 of the cannula 20. The clamping ring 172 includes clamp arms 173a, b at the free ends of the ring. The clamp arms 173a, b define a slot 174 (see FIG. 17) therebetween.

The clamping ring 172 is integral with a support column 176 forming part of the scope body 171. A column slot 177 is formed in the support column 176, with the column slot 177 being contiguous with the slot 174 between the clamp arms 173a, b. As described in more detail herein, the slots 174 and 177 permit the clamp arms 173a, b to be compressed toward each other to thereby compress the clamping surface 175 of the ring 172 about the outer surface 23 of the cannula 20. In this manner, the fixture 170 can be affixed at a specific position on the cannula 20. It is understood that when the clamping ring 172 is loosened, the fixture 170 is free to rotate about the circumference of the cannula 20 in the direction of the arrow N. In addition, the fixture 170 can translate along the longitudinal length of

the cannula 20 in the direction of the arrow T. Of course, the direction of the travel distance of the fixture 170 along the length of the cannula 20 is limited by the proximal end 22 and the bracket 27 used to engage a supporting flexible arm 160 as described above.

5 Returning to FIGS. 13-17, additional details of the fixture 170 can be discerned. In particular, the fixture 170 includes an optics mounting body 178 that is supported by and preferably integral with the support column 176. The optics mounting body 178 defines a stop edge 179 at the interface between the support column 176 and the mounting body 178. This stop edge defines the height of the support column from the clamping ring 172 to the stop edge 179. The stop edge 10 179 of the optics mounting body 178 can be used to limit the downward travel of the fixture 171 in the direction of the arrow T, which can be particularly important in embodiments of the cannula 20 that do not include the bracket 27.

 In accordance with the present embodiment, the optics mounting body 178 15 defines an optics bore 180 which is configured to receive and support an optics cannula 190. The optics bore 180 can communicate with an illumination port 181 which can receive an illumination source, such as a fiber optic light cable. The optics bore 180 also communicates with an optics coupling bore 182 projecting from a front face of the fixture 170. In accordance with one specific embodiment, 20 the fixture 170 also includes a coupling body 183 that is preferably press-fit within the optics coupling bore 182. As shown in FIG. 15, the coupling body 183 can be engaged by a coupler 184 to support a camera 185 thereon.

 In a further aspect of the optics mounting body 178, an aspiration port 186 and an irrigation port 187 can be provided that communicates with the optics bore 25 180. Preferably, the optics cannula 190 includes channels along its length to correspond to the various ports in the optics mounting body 178. In one specific embodiment, the port 181 is not used, with the port 186 being used to receive an illumination element. As shown more particularly in FIG. 23, the port 187 can be connected to an aspiration circuit. In particular, the port 187 can be engaged to an 30 aspiration tube 225 which carries a flow control valve 226 and Luer® fitting 227 at its free end. The Luer® fitting 227 can engage a source of irrigation fluid or

aspiration vacuum pressure depending upon the particular use envisioned for the port 187 and a corresponding channel within the optics cannula 190.

In accordance with a method of the present invention, the port 187 is used as an aspiration port with the Luer[®] fitting 227 connected to a vacuum source. It is understood that the port 187 is in fluid communication with a corresponding channel in the optics cannula 190 so that suction applied through the tube 225 and port 187 is drawn through the distal or working end 192 of the optics cannula 190. The working end 192 is at the surgical site so that the suction draws air through the working channel 25 of the cannula 20, to the surgical site and through the aspiration/irrigation channel in the optics cannula 190. It has been found that providing aspiration suction in this manner eliminates smoke that may be developed during operation of certain instruments, such as a Bovie. Moreover, the suction applied through the port 187 can draw air across the lens 191 (see FIG. 14, 15) of the optics cannula 190, to prevent fogging of the lens. If a separate aspiration tube is extended through the working channel, defogging of the lens 191 is best achieved with the opening of the aspiration tube adjacent the lens. In this manner, the provision of aspiration vacuum through the working channel and working space virtually eliminates the need to retract the optics cannula 190 to clean the lens 191. This is in contrast to prior devices in which either the lens had to be removed from the surgical site for cleaning or devices in which substantial flow of fluid is required to keep the lens clean and clear.

Looking now to FIGS. 18-22, details of a barrel clamp mechanism 195 are shown. The barrel clamp mechanism 195 compresses the arms 173a, b of the clamping ring 172 together to clamp the fixture 170 to the cannula 20. The barrel clamp mechanism 195 includes a barrel cam 196 disposed immediately adjacent one of the clamp arms 173b, and a lever arm 197 that operates to compress the barrel cam 196 against the clamp arm 173. A shoulder screw 198 fixes each of these components together. Specifically, the shoulder screw 198 includes a threaded shank 199 that is configured to engage a mating threaded bore 202 in one of the clamp arms 173a. The shoulder screw 198 includes a bearing shank 200 that is smooth or non-threaded. The bearing shank 200 is received within a bearing

bore 203 in the clamp arm 173b, a colinear bearing bore 204 in the barrel cam 196, and a bearing bore 205 in the lever arm 197. The shoulder screw 198 further includes an enlarged head 201 which is preferably received within a head recess 206 in the lever arm 197 (see FIG. 19). Preferably, the enlarged head 201 of the
5 shoulder screw includes a driving tool recess to mate with a driving tool to thread the threaded shank 199 of the screw into the mating threaded bore 202 of the clamp arm 173a. It is understood that the barrel cam 196 and lever arm 197 are free to rotate about the bearing shank 200 of the shoulder screw 198.

Referring specifically to FIGS. 18-19, the lever arm 197 includes an arm
10 210 that is integral with a body 211. The bearing bore 205 and head recess 206 are defined in the body 211. The body 211 defines a pair of projections 212 on opposite sides of the bearing bore 205. As depicted in FIG. 19, each of the projections 212 includes a rounded tip 213 to provide a smooth sliding surface.

Referring specifically to FIGS. 20-21, the barrel cam 196 includes a flat
15 face 215 that faces the clamp arm 173b. Preferably, the flat face provides for smooth rotation of the barrel cam 196 relative to the stationary arm 173b. The opposite face of the barrel cam 196 is a cam face 216 that includes a pair of diametrically opposite cam portions 217. In accordance with the preferred embodiment, the cam portions 217 define a ramp 218 that is inclined upward to a
20 detent recess 219. Each detent recess 219 terminates in a stop 220 that is higher relative to the base detent recess 219 than the ramp 218.

In the assembled configuration, the barrel clamp mechanism 195 operates to compress the arms 173a, b of the clamping ring 172 together when the lever arm 197 is rotated about the shoulder screw 198. Specifically, as the lever arm 197 is
25 rotated, the projections 212 slide on their rounded tip 213 along the ramps 218 until the rounded tips 213 fall within the opposite detents 219. As the projections 212 move up the ramps 218, the projections 212 push the barrel cam 196 toward the clamp arms 173a, b. More specifically, since the opposite clamp arm 173a is held relatively fixed by the threaded shank 199 of the shoulder screw 198, the
30 movement of the barrel cam 196 presses the clamp arm 173b against the relatively stationary clamp arm 173a. As this occurs, the clamping ring 172 is tightened

around the outer surface 23 of the cannula 20. When the projections 212 are seated within the recesses 219 of the barrel cam 196, the fixture is locked onto the cannula 20. It is understood that the recesses 219 are shallow enough to permit ready manual disengagement of the projections 212 from the recesses 219 as the lever arm 197 is rotated in the opposite direction.

In one specific embodiment, the detent recesses 219 are 180° opposite each other. The ramps 218 are curved and subtend an angle of about 90°. Thus, the lever arm 197 rotates through 90° to move the projections 212 from one end of the cam ramps 218 to the recesses 219. In the preferred embodiment, the lever arm ninety degree movement (arrow J in FIG. 15) moves the arm from a first position in which the arm 197 is substantially parallel to the cannula, to a second position in which the arm is substantially perpendicular to the cannula. Most preferably, in the second position the arm is oriented immediately adjacent the cannula, rather than projecting away. In the first and second positions, the lever arm 197 maintains a low profile so as not to interfere with the surgeon's manipulation of tools and instruments through the working channel. In a specific embodiment, the first position of the lever arm corresponds to the loose or unlocked position of the barrel clamp mechanism 195, while the second position corresponds to the locked configuration.

In order for the barrel clamp mechanism 195 to function properly, it is preferred that the barrel cam 196 remain stationary relative to the moveable lever arm 197, with the exception that the barrel cam 196 is free to translate along the length of the shoulder screw 198. Consequently, the clamp arm 173b includes a recess 222 that has a configuration substantially similar to the outer periphery of the barrel cam 196. In this manner, the barrel cam can be slightly indented within the clamp arm 173b so that the cam is unable to rotate about the shoulder screw 198 as the lever arm 197 is pivoted.

In accordance with one specific embodiment of the invention, the components of the fixture 170 are formed of a flexible and resilient material. For example, the scope body 171 can be formed of a plastic, such as polycarbonate. The scope body 171 lends itself particularly well to typical plastic molding

techniques. Likewise, the barrel cam 196 and lever arm 197 can be molded from a plastic material. In one specific embodiment, these components are formed of Delrin®, since Delrin® provides a smooth surface for the relative movement between the projection 212 on the lever arm 197 and the cam face 216 of the barrel cam 196.

It is understood that the travel of the barrel clamp mechanism 195 can be calibrated sufficient to tightly compress the clamping rings 172 about the cannula 20. It is also understood that this compression must not be so great as to compromise the integrity or strength of the cannula 20. In one specific embodiment, the slot 174 is larger than the maximum travel of the barrel clamp mechanism 195 so that the projections 212 of the lever arm 197 can rest solidly within the detent recesses 219 of the barrel cam 196. In accordance with one specific embodiment, the slot 174 has a dimension of 2.0mm while the throw of the barrel clamp mechanism 195 achieved by the barrel cam 196 is 1.0mm.

In accordance with the present embodiment of the invention, the fixture 170 supports an optics cannula 190 in a fixed orientation relative to the scope body 171. In other words, in this specific embodiment, the optics cannula 190 is not permitted to rotate about its axis as could the scope 50 of the embodiment shown in FIG. 1. The lens 191 is therefore mounted at an angle B relative to the distal end of the optics cannula 190. In one specific embodiment, the lens 191 is situated at an angle B of 30°. In addition, in the specific embodiment, the lens has an optical axis that is angled toward the center of the working space 25 or the cannula 20. While the lens 191 has a fixed orientation relative to the scope body 171, the lens can still be rotated around the working space by rotation of the fixture 170 about the outer surface 23 of the cannula 20. In addition, the lens 191 and the optical system provide a depth of field of view that allows the surgeon to view anatomy outside the working channel 25.

Even in the present specific embodiments, the fixture 170 allows rotation of the optics cannula 190 around the working space and translation of the optics cannula 190 and 191 along the longitudinal axis of the working channel 25. Of course, it is understood that the surgeon can achieve these motions by releasing the

barrel clamp mechanism 195 and then re-engaging the clamp by rotating the lever arm 197 to its locked position. Preferably, the optics cannula 19 is sized so that the lens 191 can project beyond the distal end 21 of the cannula 20. Similarly, in the preferred embodiment, the fixture 170 allows the retraction of the lens 191 and optics cannula 190 within the working channel 25 and cannula 20.

In one specific embodiment, the fixture 170 permits up to 15mm travel along the direction of the arrow T with 7.5mm of the travel being within the working space 25 and 7.5mm of the travel being beyond the distal end 21 of the cannula 20. In accordance with the specific embodiment, this 15mm travel distance is related to the height of the support column 176 from the top of the clamping ring 172 to the stop edge 179 of the optics mounting body 178. The amount of extension of the lens 191 of the optics cannula 190 beyond the distal end 21 of the cannula 20 is also based upon the overall length of the optics cannula 190 relative to the overall length of the working channel cannula 20. In one specific embodiment, the optics cannula 190 has a length of 100mm measured from the lens 191 to the stop edge 179 of the optics mounting bore 178. Of course, it is understood that the optics cannula is longer than this 100mm distance because a portion of the cannula is supported within the optics bore 180 of the optics mounting body 178. Again in the specific embodiment, the cannula 20 has an overall length of 92mm from its distal end 21 to its proximal end 22 (see FIG. 15).

In a further aspect of the invention, the overall length of the cannula, and consequently the optics cannula 190, is determined, in part, by the spinal anatomy. In particular, for applications of the present invention in the field of spinal surgery, it has been found that placement of the proximal end 22 of the working channel 25 too distant from the surgical site at the distal end 21 causes the surgeon to lose tactile feel while manipulating certain instruments. In other words, when the surgeon passes instruments through the working channel and manipulates them at the surgical site, a certain amount of "feel" is required so that the surgeon can accurately perform the respective operations with the instrument. If the distance between the surgical site and manual end of the instrument is too great, the surgeon will not be able to stably and comfortably operate the instrument.

In accordance one beneficial aspect of the present invention, it has been found that the working channel cannula 20 must have a length that is limited relative to the distance L (FIG. 24) between the vertebral laminae and the surface of the skin. In the lumbar region of the spine, this distance is approximately 65-75mm. Consequently, in one embodiment of the invention, the working channel cannula 20 has first portion of its length somewhat less than the anatomic distance. In one specific embodiment, this length of the first portion is about 66mm from the distal end 21 to the mounting bracket 27. In some surgical applications, the mounting bracket 27 may actually rest against the skin of the patient so that the distal end 21 of the working channel cannula can be closer to the surgical site.

Further in accordance with the present invention, the remaining second portion of the length of the cannula 20 above the mounting bracket 27 is minimized. In accordance with the invention, this distance must be sufficient to permit extension and retraction of the lens 191 relative to the distal end 21 of the cannula 20. As described above, the travel of the optical lens 191 is preferably 15mm, so that the remaining length of the cannula 20 is about 26mm to accommodate this travel and to provide adequate surface for engagement by the clamping rings 172. Thus, in the preferred embodiment, the working channel cannula 20 has an overall length of 92mm. In accordance with one aspect of the invention, it has been found that the relative length between the first portion of the cannula disposed within the patient to the second portion of the cannula length situated outside the patient have a ratio of 2:1 to 3:1. In other words, the length of the first portion is between two to three times longer than the length of the second portion.

It has also been found that it is desirable to minimize the height of the fixture 170 beyond the end of the working channel cannula 20. In accordance with the present invention, the optics mounting body 178 has a height of about 21mm between the stop edge 179 and the top face of the body 178. This distance is not so great that the surgeon has restrained from manipulating instruments directly above the fixture 170. Of course, it is preferable that the surgeon manipulate the

instruments directly above the proximal end 22 of the working channel 20 immediately adjacent to the fixture 170.

In the present preferred embodiment, the working channel cannula has an inner diameter of about 15mm and an outer diameter of about 16mm.

5 Alternatively, the cannula can be provided in a smaller size for other regions of the spine. In a further specific embodiment, the cannula inner diameter is 12.7mm with a 14mm outer diameter. In another aspect of the invention, the overall length and diameter of the working channel cannula 20 is calibrated again relative to the distance L of the spinal anatomy. With the larger diameter working channel, the
10 surgeon can orient certain instruments at an angle relative to the longitudinal axis of the cannula 20. In specific embodiments, this angle is approximately 5-6°. It has been found that this angle, together with the large working channel 25, gives the surgeon greater flexibility and mobility within the surgical site to perform various operations. To that end, the length and diameter of the working channel
15 cannula 20 is appropriately sized to maintain this flexibility, without getting too large. A working channel cannula 20 that has too large a diameter is less adaptable to the spinal anatomy.

In accordance with preferred methods using the devices of the present invention, the working space is generally limited to the region directly adjacent the
20 laminae of a vertebra. A cannula having a diameter that is too large will interfere with the spinous process when the working space is created, and will require resection of greater amounts of tissue than is preferred for an optimal percutaneous procedure. Therefore, in accordance with one aspect of the invention, the working channel cannula has a relationship between its length and its diameter to permit
25 tool angles through the cannula of between 5-8°. In accordance with one specific aspect of the present invention, the cannula can have a length to diameter ratio of between about 5.5:1 to 7:1. Further in accordance with the present invention, the working channel cannula has a length that is no more than 20-30mm greater than the distance L (FIG. 24) between the laminae and the skin of the patient.

30 One important feature of the present invention is achieved by the large diameter of the working channel 25 in the cannula 20. This large diameter allows

the surgeon or surgeons conducting the surgical procedure to introduce a plurality of instruments or tools into the working space. For example, as described above, a tissue retractor and discectomy instruments can be simultaneously extended through the working channel. In the illustrated embodiment, the discectomy
5 instruments could include a trephine for boring a hole through the disc annulus and a powered tissue cutter for excising the herniated disc nucleus. Likewise, the present invention contemplates the simultaneous introduction of other types of instruments or tools as may be dictated by the particular surgical procedure to be performed. For example, an appropriately sized curette and a rongeur may be
10 simultaneously extended through the working channel into the working space. Since all operations being conducted in the working space are under direct visualization through the viewing element, the surgeon can readily manipulate each of the instruments to perform tissue removal and bone cutting operations, without having to remove one tool and insert the other. In addition, since the surgical
15 procedures can be conducted without the necessity of irrigation fluid, the surgeon has a clear view through the working space of the target tissue. Furthermore, aspects of the invention which permit a wide range of motion to the viewing element allow the surgeon to clearly visualize the target tissue and clearly observe the surgical procedures being conducted in the working space.

20 The surgeon can capitalize on the same advantages in conducting a wide range of procedures at a wide range of locations in the human body. For example, facetectomies could be conducted through the working channel by simply orienting the working channel cannula 20 over the particular facet joints. The insertion of vertebral fixation elements can also be accomplished through the devices. In this
25 type of procedure, an incision can be made in the skin posterior to the location of the vertebra at which the fixation element is to be implanted. Implementing the steps shown in FIG. 10, the cannula 20 can be positioned through the incision and tissue directly above the particular location on the vertebra to be instrumented. With the optics extending through the working channel, an insertion tool holding
30 the vertebral fixation element can be projected through the cannula 20 and manipulated at the vertebra. In one specific embodiment, the fixation element can

be a bone screw. The working channel 25 has a diameter that is large enough to accept most bone screws and their associated insertion tools. In many instances, the location of the bone screw within the vertebra is critical, so identification of the position of the cannula 20 over the bony site is necessary. As mentioned above,
5 this position can be verified fluoroscopically or using stereotactic technology.

In many prior procedures, cannulated bone screws are driven into the vertebra along K-wires. The present invention eliminates the need for the K-wire and for a cannulated screw. The working channel itself can effectively operate as a positioning guide, once the cannula 20 is properly oriented with respect to the
10 vertebra. Moreover, the devices allow insertion of the bone screw into the vertebra to be conducted under direct vision. The surgeon can then readily verify that the screw is passing into the vertebra properly. This can be particularly important for bone screws being threaded into the pedicle of a vertebra. The working channel cannula 20 can be used to directly insert a self-tapping bone screw into the pedicle,
15 or can accept a variety of tools to prepare a threaded bore within the pedicle to receive a bone screw.

The devices can also be used to prepare a site for fusion of two adjacent vertebrae, and for implantation of a fusion device or material. For example, in one surgical technique, an incision can be made in the skin posterior to a particular disc
20 space to be fused. The incision can be made anteriorly, posteriorly or posterior laterally. If the incision is made anteriorly for anterior insertion of the working channel, it is anticipated that care will be taken to retract tissues, muscle and organs that may follow the path of the incision to the disc space. However, the devices of the present invention allow this tissue retraction to occur under direct
25 vision so that the surgeon can easily and accurately guide the cannula 20 to the disc space without fear of injury to the surrounding tissue. As the tissue beneath the skin is successively excised or retracted, the working channel cannula 20 can be progressively advanced toward the anticipated working space adjacent the vertebral disc. Again under direct vision, the disc space can be prepared for
30 implantation of fusion materials or a fusion device. Typically, this preparation

includes preparing an opening in the disc annulus, and excising all or part of the disc nucleus through this opening.

In subsequent steps, a bore is cut through the disc annulus and into the endplates of the adjacent vertebrae. A fusion device, such as a bone dowel, a push-in implant or a threaded implant can then be advanced through the working
5 channel of the cannula 20 and into the prepared bore at the subject disc space. In some instances, the preparatory steps involve preparing the vertebral endplates by reducing the endplates to bleeding bone. In this instance, some aspiration and irrigation may be beneficial. All of these procedures can be conducted by tools
10 and instruments extending through the working channel cannula 20 and under direct vision from the viewing element.

In some instances, graft material is simply placed within the prepared bore. This graft material can also be passed through the working channel cannula 20 into the disc space location. In other procedures, graft material or bone chips are
15 positioned across posterior aspects of the spine. Again, this procedure can be conducted through the working channel cannula particularly given the capability of the cannula to be moved to different angles from a single incision site in the skin.

The present invention provides instruments and techniques for conducting a variety of surgical procedures. In the illustrated embodiments, these procedures
20 are conducted on the spine. However, the same devices and techniques can be used at other places in the body. For example, an appropriately sized working channel device 10 can be used to remove lesions in the brain. The present invention has particular value for percutaneous procedures where minimal invasion into the patient is desirable and where accurate manipulation of tools and
25 instruments at the surgical site is required. While the preferred embodiments illustrated above concern spinal procedures, the present invention and techniques can be used throughout the body, such as in the cranial cavity, the pituitary regions, the gastro-intestinal tract, etc. The ability to reposition the viewing optics as required to visualize the surgical site allows for much greater accuracy and control
30 of the surgical procedure. The present invention allows the use of but a single

entry into the patient which greatly reduces the risk associated with open surgery or multiple invasions through the patient's skin.

In accordance with yet another aspect of the present invention, a tissue retractor apparatus 230 is provided that combines a tissue retractor 231 with an optical viewing device 232. Referring to FIGS. 25-26, the retractor apparatus 230 includes a retractor plate 234 that is affixed to a grip 235 for manual support of manipulation of the retractor. The grip 235 is at the proximal end 236 of the plate. The distal end 237 of the retractor plate preferably has a blunt tip 238 to avoid trauma upon insertion and manipulation of the tissue retractor. Preferably, the blunt tip 238 is angled slightly away from the plate 234. The retractor plate 234 defines an outer retraction surface 239 that can be configured according to the type of surgery being performed. In a preferred embodiment, the plate 234 is semi-cylindrical in configuration to permit atraumatic retraction of tissue adjacent a surgical site. In addition, the retractor plate 234 defines a channel 240 that helps define a working channel. As thus far described, the retractor 231 is substantially similar to the retractor 70 depicted in FIGS. 4-6 and as described above.

In accordance with this embodiment of the invention, an optical viewing device 232 is supported within the retractor 231 by way of a number of C-clips 245. Preferably, the C-clips 245 are formed of a resilient material, such as plastic or thin flexible metal, and are affixed to the channel 240 of the retractor plate 234. In accordance with one specific embodiment, two such C-clips 245 are provided to stably mount the optical viewing device 232 relative to the retractor 231. Preferably, the clips 245 are sized to support an optical viewing device 232 that is configured substantially identical to the viewing device 50 described above. In the preferred embodiment, the viewing device 232 has a distal tip 52 with an angled lens 54. In accordance with this embodiment, the C-clips 245 provide a resilient friction fit to the optical viewing device 232 while still permitting relative sliding and rotation of the viewing device 232 relative to the retractor 231.

In accordance with the present invention, the tissue retractor apparatus 230 can be used in a variety of applications, including non-spinal applications. For example, this tissue retractor can have application in transnasal and transphenoidal

surgeries, and in pituitary procedures. In surgeries of this type, it is not necessarily desirable to provide a closed cannula, such as a working channel cannula 20. Moreover, the smaller working space does not lend itself to the use of a closed cannula which would tend to restrict the space available for manipulation of surgical instruments. Consequently, a tissue retractor or speculum of the type
5 shown in FIGS. 25-26 may be very adequate for surgeries of this type. In this instance, then the working channel is defined in part by the patient's body itself, and in part by the tissue retractor. The optical viewing device 232 is supported relative to the retractor to permit the same degrees of motion as are available with
10 the device 10 described above.

In another embodiment of the invention and referring to FIG. 27, a modular clamp assembly 300 for supporting viewing optics and/or irrigation/aspiration components is provided with the cannula 20. This embodiment is mounted on a cannula 20 having features similar to those previously described, and similar
15 features are referenced by the same numerals. In accordance with this embodiment, the assembly 300 is provided with a viewing element 310 and a clamp assembly 350, which are shown most clearly in FIGS. 28, 29, and 30. The viewing element 310 includes a viewing portion 312 and an illumination element 314 coupled to a body portion 316. As shown more clearly in FIG. 28, body
20 portion 316 has an optics cannula 320 and dovetail 330 extending therefrom towards the cannula 20 when placed thereon. Preferably, dovetail 330 is integrally formed with the body portion 316. When engaged to the cannula 20, optics cannula 320 extends from a proximal end 22 of cannula 20 to distal working end 21, as shown in FIG. 27.

25 In the embodiment of the present invention, illustrated in FIG. 27a, the distal working end 21 is beveled and includes a cutting edge 302 for penetrating bone and soft tissue. A sloped retraction surface 304 extends from edge 302 to outer surface 23 of cannula 20. Retraction surface 304 acts to gradually separate tissue while minimizing damage thereto as the cannula is advanced to the desired
30 depth at the surgical site.

Body portion 316 defines an optics bore (not shown) for receiving and supporting optics cannula 320, and to provide visual communication to viewing portion 312. In one embodiment, the optics bore communicates with illumination element 314, which is configured to communicate with an illumination source. In a preferred embodiment, components of the viewing portion 312, such as the eyepiece component 326 and focus adjustment knob 327, are integrally formed with the body portion 316. In an alternate embodiment, the viewing portion 312 is threadingly coupled to body portion 316.

Referring now to the clamp assembly 350, there is included a clamp ring 352 and a viewing element receiving portion 390 extending from clamp ring 352. Receiving portion 390 defines a dovetail receptacle 396 for receiving an insertion end 332 of dovetail 330 in sliding engagement. It should be understood that the receptacle 396 may alternately be defined by body portion 316 of viewing element 310, and dovetail 330 may extend from receiving portion 390 to engage the receptacle 396.

Clamp ring 352 substantially encircles an outer surface 23 of cannula 20. In particular, clamp ring 352 includes a clamping surface 356 (see FIG. 28). In a preferred embodiment, clamping surface 356 has substantially the same configuration and dimension as outer surface 23 of cannula 20. The clamping ring 352 includes clamping arms 354a and 354b at the free ends of the ring 352. The clamping arms 354a and 354b define a slot 358 therebetween. As described below in more detail, the slot 358 permits arms 354a and 354b to be compressed toward each other to thereby compress clamping surface 356 of the ring 352 about the outer surface 23 of the cannula. It is understood that when clamping ring 352 is loosened, the clamp assembly 350, and if engaged thereto, the viewing element 310 are free to rotate about the circumference of the cannula 20 in the direction of arrow N. Additionally, the clamp assembly 350 can translate along the longitudinal length of the cannula 20 in the direction of the arrow T. The length of travel is limited by the bracket 27 used to engage the flexible support arm 160 as described previously.

Extending from and integrally formed with clamp ring 352 is receiving portion 390. In a preferred embodiment, receiving portion 390 includes a surface 392 that abuttingly engages a stop surface 328 of body portion 316 when dovetail 330 is fully received within receptacle 396. In one embodiment, stop surface 328 of the viewing element 310 limits the downward travel of the assembly 300 along the cannula 20 by engaging proximal end 22 of cannula 20.

In a further aspect of the clamp assembly 350, an irrigation port 393, shown in FIG. 29, can be provided through receiving portion 390 to allow connection of irrigation cannula 324 to an irrigation tube 225b via irrigation port 393. Luer® lock fitting 227b couples tube 225b to an irrigation source (not shown). An aspiration port 392 may also be provided through clamp assembly 350 to allow connection of aspiration cannula 322 to an aspiration tube 225a through aspiration port 392. Luer® lock fitting 227a couples tube 225a to an aspiration source (not shown). It should be understood that the clamp assembly 350 may be provide with both an irrigation cannula 324 and an aspiration cannula 322 with corresponding ports 393 and 392 through receiving portion 390. In one embodiment, only one of the irrigation/aspiration cannulas and its corresponding port is provided. In another embodiment, no irrigation or aspiration cannulas or ports are provided. In yet another embodiment, a single irrigation/aspiration cannula and port is provided and irrigation and aspiration is performed alternately through the single tube and port. It should be understood that the irrigation/aspiration cannula(s) may be used according to the methods described above.

Clamp assembly 350 and viewing element 310 are releasably engaged via connection assembly 318. Connection assembly 318 is shown to be preferably positioned on clamp assembly 350; however, it should be understood that in alternate embodiments connection assembly 318 may be provided on viewing element 310. Referring now to FIG. 31, connection assembly 318 includes a clip 340 pivotably mounted to viewing element receiving portion 390 of clamp assembly 350 via resilient hinges 345. In the illustrated embodiment, clip 340 is mounted via two resilient hinges 345. In an alternate embodiment, only one hinge 345 is used to mount clip 340.

Resilient hinge 345 biases clip 340 to a position, as shown in FIG. 31, where the body of clip 340 is substantially parallel to body portion 316 and receiving portion 390. A protuberance 335 projects from and is preferably integrally formed with body portion 316 of viewing element 310. Clip 340 defines
5 an aperture 342, 343 configured and positioned to receive protuberance 335 when dovetail 330 is fully received within receptacle 396, placing the viewing element 310 and the clamp assembly 350 in an assembled position (as shown in FIG. 27.) In the assembled position, stop surface 328 is proximate engagement surface 392. In one embodiment, stop surface 328 engages engagement surface 392. In another
10 embodiment, a space is left between stop surface 328 and engagement surface 392 when the viewing element 310 is coupled to clamp assembly 350.

Clip 340 has a first end 346 defining a nose portion 344 extending toward viewing element 310 when it and clamp assembly 350 are positioned as shown in FIG. 28. Protuberance 335 defines an inclined surface 336 that opposes nose
15 portion 344. Nose portion 344 slidably engages the inclined surface 336 as dovetail 330 is placed in receptacle 396. This protuberance acts as a cam to rotate the nose portion 344 as it moves along inclined surface 336, causing the clip 340 to rotate in a direction indicated by arrow P. As the dovetail 330 is further positioned within receptacle 396, the wall 343 of aperture 342, 343 eventually communicates
20 with engagement surface 337 of protuberance 335. Hinge 345 then biases the clip 340 to the position shown in FIG. 31, where the engagement surface 337 engages an endwall 343 that defines a portion of the aperture 342, 343.

Once coupled the viewing element 310 and clamp assembly 350 are effectively held in such position by the clip 340. In order to uncouple the
25 scope/clamp assembly, clip 340 is rotated by depressing second end 347 via handle portion 341 in the direction of arrow "P" to rotate the clip 340 about hinge 345. Nose portion 344 is thus rotated in the direction opposite arrow P until endwall 343 no longer engages engagement surface 337. The viewing element 310 may then be removed from the clamp assembly 350 by sliding dovetail 330 out of the receptacle
30 396.

It should be understood that the present invention contemplates other structures for coupling viewing element 310 to clamp assembly 350. For example (by way of illustration and not limitation), dovetail 330 may be replaced by one or more guide pins extending from viewing element 330 to be received within
5 corresponding slots on receiving portion 390. Alternatively, the clip 340 may be provided on one or both of the side portions of the receiving portion 390.

With reference now to FIG. 32, there is illustrated a plan view of clamp assembly 350 and a portion of a section through viewing element 310. Clamp assembly 350 is shown removed from cannula 20 for clarity. Dovetail 330 is
10 shown positioned within receptacle 396, and protuberance 335 is received within the aperture 342, 343 of clip 340. Receiving portion 390 further defines an optics recess 359 for receiving optics cannula 320 between irrigation port 393 and aspiration port 394. Optics recess 359 allows placement of the optics cannula 320 adjacent the working channel 25 of the cannula 20.

15 The clamp assembly 350 may be loosened and rotated or translated about the cannula 20 via the lever arm assembly 360, shown in exploded view in FIG. 32. Lever arm assembly 360 includes fastener 380 coupling a lever arm 366 to clamping arms 354a and 354b. Fastener 380 includes an enlarged head 381, a shank portion 382 integrally formed therewith and extending therefrom. Shank
20 portion 382 defines a threaded portion 383 remote from the head 381.

Lever arm 366 has a first end 369 and a second end 371. In proximate second end 371 there is a portion of a bearing bore through lever arm 366 which has a shank receiving portion 372 and a colinear head receiving portion 375. Lever arm 366 also includes an inside face 367 adjacent arm 354b. Projecting from face
25 367 and integrally formed therewith is cam portion 364. Referring to FIG. 33, cam portion 364 has one or more arcuate inclined ramps 377a, 377b, 377c, 377d, collectively designated as ramps 377. Each ramp 377 is inclined upward from a low portion 378 to a high portion 379. Between low portions 378 and high portions 379 of adjacent ramps 377 are detents 374.

30 Referring back to FIG. 32, clamping arms 354a and 354b have a bore 361 which includes a threaded portion 368 in arm 354a, and the other portion of the

bearing bore having a bearing portion 370 and a colinear shank receiving portion 372 in arm 354b. Arm 354b also includes projections 362a and 362b extending therefrom and integrally formed therewith. Projections 362a and 362b are configured to releasably engage and be received within a corresponding one of the
5 detents 374.

When lever arm assembly 360 is assembled, threaded portion 383 of fastener 380 threadingly engages clamp arm 354a to secure lever arm 366 thereto. Shank portion 382 is rotatably received within shank receiving portions 372, and head 381 is received within head receiving portion 375. By rotating lever arm 366
10 about shank 382 of fastener 380, lever arm 366 is operable to selectively compress or release arms 354a and 354b to allow clamping surface 356 to engage outer surface 23 of cannula 20. Thus rotation of the assembly 300 is accomplished in the N direction or translation in the T direction (FIG. 27) along cannula 20 by releasing clamping ring 352. In order to release clamp ring 352, lever arm 366 is
15 positioned so that projections 362 releasably engage a corresponding one of detents 374 adjacent low portions 378. It is understood that the detents 374 are configured to allow disengagement of projections 362 by a reasonable force applied to first end 369 of lever arm 366. Once clamp ring 352 is in the desired position, the lever arm 366 is rotated so that the projections slide up corresponding ones of the ramps
20 377 until the projection falls into a detent between the high portions 379 of adjacent ramps 377, thus compressing and then holding clamp ring 352 about the outer surface 23 of the cannula 20.

FIG. 34 illustrates an alternate configuration cam 364' of lever arm 366. In this embodiment, there is provided two ramps 377a and 377b. Adjacent high
25 portions 379a, 379b of each ramp 377a, 377b is a corresponding detent 374a, 374b, respectively. Stops 386a and 386b are provided adjacent a corresponding one of the detents 374a, 374b opposite the high portions 379a, 379b. A first side 387a, 387b of stops 386a, 386b is configured to prevent detents 374a, 374b from being rotated past projections 362 when clamp 352 is clamped to the cannula 20. When
30 the lever arm 366 is manipulated to release projections 362 from the detents 374a, 374b in order to release clamp 352, the projections slide down ramps 377a, 377b to

inside face 367. A back side 388a, 388b of stops 386a, 386b engage the projections to limit further rotation of the lever arm 366.

In the embodiment of FIG. 33, the detents 374 are spaced at 90 degrees about the cam 364. Thus, the lever arm 366 moves through an angle of about 90
5 degrees to move the projections 362 from a detent 374 adjacent to a lower portion of the ramp to a detent 374 adjacent an upper portion of the ramp. In the embodiment of FIG. 34, the detents 374 are spaced at 180 degrees, but the inclined ramps 377a and 377b terminate upon turning through an arc of about 90 degrees. Preferably, when clamp ring 352 is engaged to cannula 20, lever arm 366 extends
10 perpendicular to cannula 20 and is positioned adjacent the clamp ring 352, as illustrated in FIG. 32. This minimizes the profile of clamp assembly 350 and any interference that could be caused by lever arm 366 with the surgeon's manipulation of tools and performance of surgical procedures. In one embodiment, the lever arm is rotated 90 degrees to be parallel to the cannula in order to release clamp 352
15 to reposition or remove the clamp assembly 350. In another embodiment, the clamp 352 is released when the lever arm 366 is rotated in the range of about 45 degrees to about 135 degrees from its clamped position perpendicular to the axis of the cannula 20.

Referring now to FIG. 35, another embodiment of a clamping assembly of
20 the present invention is illustrated and designated at 400. Clamping assembly 400 has a ring that includes a pair of clamping arms 402 and 404. Arms 402 and 404 are pivotably coupled with one another via clamping mechanism 401. Clamping mechanism 401 includes a pair of lever 408 and 410 coupled to hinge portion 406. Levers 408 and 410 and hinge 406 are coupled to arms 402 and 404, and allowing
25 the arms 402, 404 to be selectively engaged to the outer surface 23 of cannula 20. Clamp mechanism 400 further includes a viewing element receiving portion 412 extending from and integrally formed with one the clamping arms (shown in FIG. 35 connected to arm 402). Receiving portion 412 is similarly configured to function like viewing element receiving portion 390, as illustrated and described
30 with respect to FIGs. 28-29, with like elements being indicated by like reference numerals. Lever arm 402 defines a cannula engaging surface 416, and lever arm

404 defines a cannula engaging surface 418. Free end 403 of lever arm 492 and free end 405 of lever arm 404 define a slot or gap 419 therebetween. The size of gap 419 is not critical, so long as arms 402, 404 are operable to selectively grip the cannula 20.

5 Arms 402 and 404 are biased by a spring (not shown) coupled to hinge 406 so that clamping surfaces 416, 418 provide a gripping force against outer surface 23 of cannula 20. In order to rotate, translate, or remove the clamping mechanism with respect to the cannula 20, lever arms 408, 410 are pressed towards one another (as indicated by the arrows 408a, 410a in FIG. 35) to separate first ends 10 403 and 405. The grip of clamping surfaces 416, 418 is then released from outer surface 23, and the mechanism 400 may be moved along the length of the cannula 20 or removed from the cannula 20 according to the need of the surgeon.

 It is contemplated that hinge 406 may be any type of hinge suitable for clamping clamp mechanism 400 to cannula 20 as would occur to those skilled in 15 the art. For example, hinge 406 may include a pin extending through colinear bores defined by the clamping arms 402, 404, with a spring biasing arms 402, 404 to their clamping position.

 It should be understood that clamp assemblies 350 and 400 each allow rotation and translation of optics 190 similarly as described above with respect to 20 fixture 170.

 In accordance with one specific embodiment of the invention, portions of viewing element 310 and the components of the clamp assemblies 350 and 400 are formed of a flexible and resilient material. For example, the body portion 316 and receiving portion 390 can be formed of a plastic, such as polycarbonate, and are 25 particularly well-suited to typical plastic molding techniques. Likewise, the lever arm 366 and can be molded from a plastic material. In one specific embodiment, these components are formed of Delrin[®], since Delrin[®] provides a smooth surface for the relative movement between the projections 362 on the clamping arm 354b and the cam faces 364, 364' of lever arm 366.

30 It is understood that the travel of the barrel clamping mechanism 360 and biasing force of mechanism 401 can be calibrated so as to tightly compress the

clamping ring 352 and arms 402, 404 respectively, about the cannula 20. It is also understood that this compression must not be so great as to compromise the integrity or strength of the cannula 20. In one specific embodiment, the slot 358 is larger than the maximum travel of the barrel clamp mechanism 360 along inclined ramps 377 so that the projections 362 can rest solidly within the detents 374 of the lever arm 366. In accordance with one specific embodiment, the slot 358 has a dimension of 2.0mm while the throw of the barrel clamp mechanism 360 achieved by the cam 364 is 1.0mm.

From the foregoing description of the embodiments of the present invention illustrated in FIGs. 27-36, several advantages and methods of using the present invention should be understood. The detachability of the viewing element 310 from the clamp assemblies 350 or 400 allows multiple uses of a single viewing element 310. The same viewing element 310 may also be used with clamp assemblies manufactured for different sized and shaped cannulas. Since a single viewing element 310 may be used for multiple sized cannulas and clamp assemblies, the unit cost per procedure is reduced. Also, it is cost-effective to manufacture the viewing element and its components from high-quality materials. For example, optics cannula 320 may be made from stainless steel. High quality materials for optical components often enable the use of smaller-sized components, thus conserving additional area in the working channel of the cannula for surgical working space. In one specific embodiment, optics cannula 320 has a diameter of about 3mm. Optimum picture quality may also be obtained by use of glass components in the viewing element.

Referring now to FIGs. 36-37, alternate embodiments of cross-sections for the cannula 20 are illustrated. The cannula 20 has been illustrated with having a generally circular cross-section. It is also contemplated that the cannula 20 have non-circular cross-sections. For example, FIG. 36 cannula 430 has an outer surface 432 that defines an oval cross-section. In FIG. 37, the cannula 440 has an outer surface 442 that defines a square cross-section. Of course, it should be understood that corresponding adjustments in the design and configuration of the fixtures and clamping assemblies described herein are also required in order to

engage the outer surface of the cannulas illustrated in FIGs. 36-37. In one embodiment, the cannula 20 of the present invention has a variable cross section profile along at least a portion of its length between proximal end 22 and distal end 21. The variable profile provides a larger cross-sectional dimension and/or area at the proximal end 22 than at the distal working end 21. In one form, the variable profile defines a frusto-conical portion along longitudinal axis L of the cannula 20.

While the invention has been illustrated and described in detail in the drawings and foregoing description, the same is to be considered as illustrative and not restrictive in character, it being understood that only the preferred embodiment has been shown and described and that all changes and modifications that come within the spirit of the invention are desired to be protected.

What is claimed is:

1. An apparatus for use in percutaneous surgery, comprising:
an elongated cannula sized for percutaneous introduction into a patient, said
cannula defining a working channel and having a longitudinal axis extending
5 between a distal working end and an opposite proximal end, said cannula further
defining an outer surface thereabout;
a clamp assembly movably engaged to said cannula; and
a viewing element releasably engaged to said clamp assembly.
2. The apparatus of claim 1, wherein said clamp assembly includes a
10 viewing element receiving portion and said viewing element includes a clamp
assembly engaging portion, said receiving portion configured to releasably engage
said engaging portion.
3. The apparatus of claim 2, wherein said receiving portion defines a
receptacle and said engaging portion includes a dovetail, said dovetail configured
15 to be slidably received within said receptacle.
4. The apparatus of claim 2, wherein said viewing element includes an
optics cannula and said receiving portion defines an optics recess for receiving a
portion of said optics cannula when said viewing element is engaged to said clamp
assembly.
- 20 5. The apparatus of claim 4, wherein said optics cannula is positioned
adjacent said working channel when said viewing element is engaged to said clamp
assembly.
6. The apparatus of claim 5, wherein said clamp assembly engaging
portion includes a protuberance and said viewing element receiving portion
25 includes a clip pivotably engaged to said clamp assembly, said clip defining an
aperture for engaging said protuberance when said dovetail is received within said
receptacle.
7. The apparatus of claim 1, wherein said cannula defines a circular
cross-section.
- 30 8. The apparatus of claim 1, wherein said cannula defines a square
cross-section.

9. The apparatus of claim 1, wherein said cannula defines an oval cross-section.

10. The apparatus of claim 1, wherein said distal working end is beveled.

5 11. The apparatus of claim 10, wherein said beveled distal working end includes a cutting edge and a sloped retraction surface extending from said cutting edge to said outer surface.

12. The apparatus of claim 1, wherein said viewing element is an endoscope.

10 13. The apparatus of claim 1, wherein said viewing element is a microscope.

14. The apparatus of claim 1, further comprising a flexible arm having a first end engaged to said cannula and a second end fixedly mounted away from said cannula.

15 15. The apparatus of claim 14, further comprising a bracket having a first end engaged to said cannula and a second end engaged to said first end of said flexible arm.

16. The apparatus of claim 1, wherein said cannula is made of stainless steel.

20 17. The apparatus of claim 1, wherein said cannula is made of plastic material.

18. The apparatus of claim 1, wherein said clamp assembly comprises:
a ring sized to substantially encircle the cannula, said ring including a pair of adjacent free ends;

25 a pair of opposing arms extending from a corresponding one of said free ends, said arms defining a slot extending between said free ends;

a mechanism connected to said arms operable to compress said arms toward each; and

a viewing element receiving portion extending from said ring.

19. The apparatus of claim 18, wherein said viewing element includes a clamp assembly engaging portion, said receiving portion configured to releasably receive said engaging portion.

20. The apparatus of claim 19, wherein said receiving portion defines a
5 receptacle and said engaging portion includes a dovetail, said dovetail configured to be slidably received within said receptacle.

21. The apparatus of claim 20, wherein said clamp assembly engaging
portion includes a protuberance and said viewing element receiving portion
includes a clip pivotably engaged to said clamp assembly, said clip defining an
10 aperture for engaging said protuberance when said dovetail is received within said
receptacle.

22. The apparatus of claim 1, wherein said clamp assembly comprises:
a first arm pivotably coupled to a second arm, each of said first and second
arms configured to encircle a portion of the outer surface of said cannula and each
15 defining a free end, said free ends positioned adjacent one another;
a handle portion extending from each of said first and second arms, wherein
said first and second arms are biased against the outer surface of said cannula; and
a viewing element receiving portion extending from one of said arms.

23. The apparatus of claim 22, wherein said viewing element includes a
20 clamp assembly engaging portion, said receiving portion configured to releasably
receive said engaging portion.

24. The apparatus of claim 23, wherein said receiving portion defines a
receptacle and said engaging portion includes a dovetail, said dovetail configured
to be slidably received within said receptacle.

25. The apparatus of claim 24, wherein said clamp assembly engaging
portion includes a protuberance and said viewing element receiving portion
includes a clip pivotably engaged to said viewing element receiving portion, said
clip defining an aperture for engaging said protuberance when said dovetail is
received within said receptacle.

30 26. An assembly for supporting a viewing element adjacent a cannula,
comprising:

a ring sized to substantially encircle the cannula, said ring including a pair of adjacent free ends;

a mechanism engaged to said ring operable to bias said free ends towards one another to engage an outer surface of the cannula; and

5 a viewing element receiving portion extending from said ring.

27. The assembly of claim 26, wherein said ring includes a first arm pivotably coupled to a second arm, each of said first and second arms including a corresponding one said adjacent free ends;

28. The assembly of claim 27, wherein said mechanism further
10 includes:

a lever arm extending from each of said first and second arms; and

a hinge pivotably coupling said first and second arms, said hinge biasing said arms against the outer surface of the cannula.

29. The assembly of claim 26, further including a pair of opposing arms
15 extending from a corresponding one of said free ends, said arms defining a slot extending between said free ends; and

said mechanism connected to said arms being operable to compress said arms together.

30. The apparatus of claim 29, wherein one of said arms include at least
20 one projection extending therefrom and said mechanism includes:

a lever arm having an inside face facing said at least one projection, said inside face including a cam surface with at least one inclined ramp; and

a fastener rotatably engaging said lever arm to said pair of arms with said cam surface disposed for contact with said at least one projection,

25 whereby rotation of said lever arm relative to said pair of arms causes said at least one projection to slide along said ramp to push said pair of arms toward each other to narrow the slot.

31. The apparatus of claim 30, whereby said mechanism further
includes:

30 a threaded bore in one arm of said pair of arms;

bearing bores defined in the other arm of said pair of arms and said lever arm, said bearing bores being coaxial with said threaded bore; and

said fastener including a threaded shank for mating with said threaded bore, a non-threaded bearing shank extending through said bearing bores, and a head
5 larger than said bearing bores for engaging said lever arm when said threaded shank is engaged within said threaded bore.

32. The apparatus of claim 30, wherein said cam surface of said lever arm includes a detent at one end of said inclined ramp, said detent being sized to receive said projection therein.

10 33. The apparatus of claim 30, wherein said at least one ramp is arcuate.

34. The apparatus of claim 30, wherein said cam surface includes two inclined ramps; and

said lever arm includes two projections in sliding contact with said ramps.

35. The apparatus of claim 34, wherein said cam surface of said lever
15 arm includes a detent at an upper portion of said inclined ramps, each of said detents being sized to receive a corresponding one of said projections therein.

36. The apparatus of claim 35, wherein said cam surface further includes a stop adjacent each of said detents,

whereby said stop mechanism engages a corresponding one of said
20 projections to prevent further rotation of said lever arm.

37. The apparatus of claim 36, wherein said two detents are spaced at 180 degrees on said inside surface of said lever arm.

38. The apparatus of claim 30, wherein said cam surface includes four inclined ramps spaced thereabout, each of said ramps having a high portion
25 adjacent a high portion of one of said ramps and low portion adjacent a low portion of another of said ramps.

39. The apparatus of claim 38, wherein said cam surface defines four detents, each detent being located between corresponding adjacent ramp portions.

40. An apparatus for performing percutaneous surgery, comprising:
30 a cannula having a distal working end and a proximal end and defining a working channel therethrough, said cannula having an outer surface thereabout;

a bracket having a first end and an opposite second end, said first end engaged to said outer surface of said cannula; and

a flexible arm having a first end and an opposite second end, said first end of said flexible arm engaged to said second end of said bracket, said second end of
5 said flexible arm being securely mounted away from the surgical site.

41. The apparatus of claim 40, wherein said flexible arm is contoured.

42. The apparatus of claim 40, further including a clamp assembly movably engaged to said cannula; and

a viewing element releasably engaged to said clamp assembly.

10 43. The apparatus of claim 42, wherein said clamp assembly includes a viewing element receiving portion and said viewing element includes a clamp assembly engaging portion, said receiving portion configured to releasably receive said engaging portion.

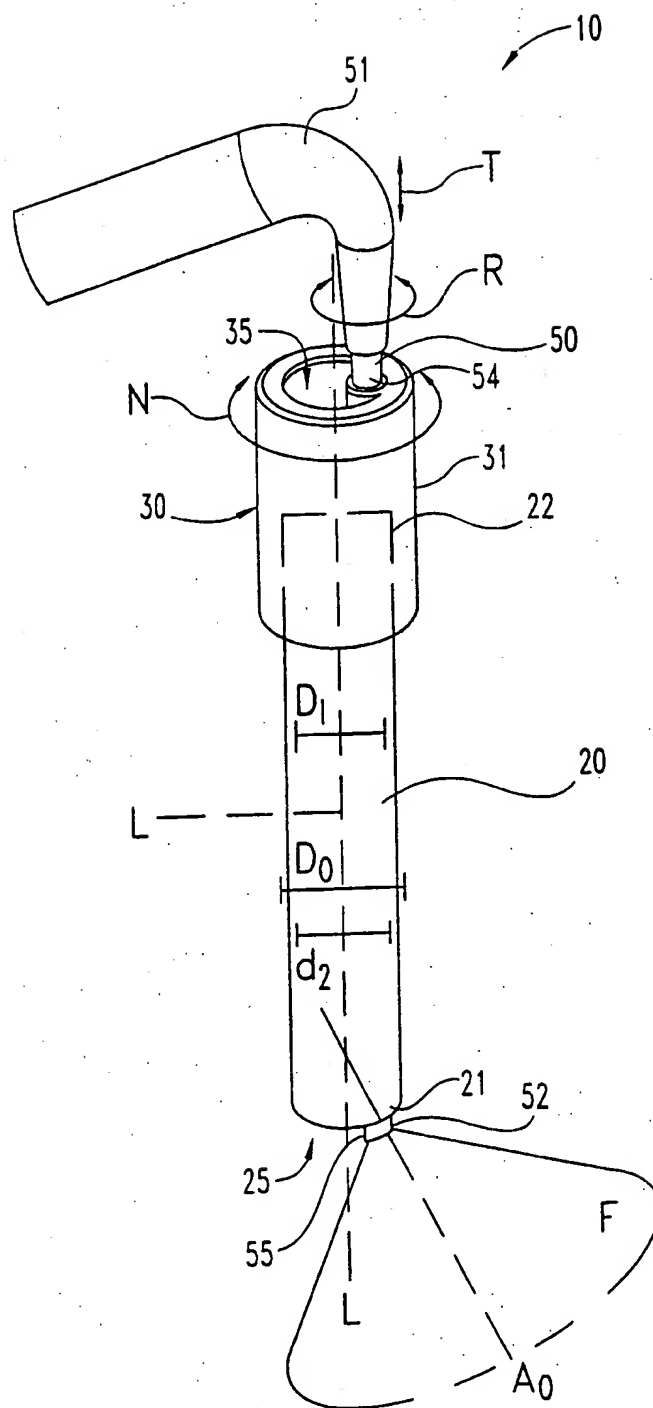


Fig. 1

2/21

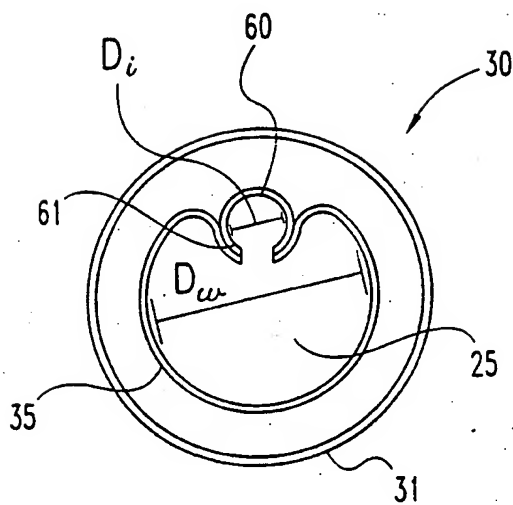


Fig. 2

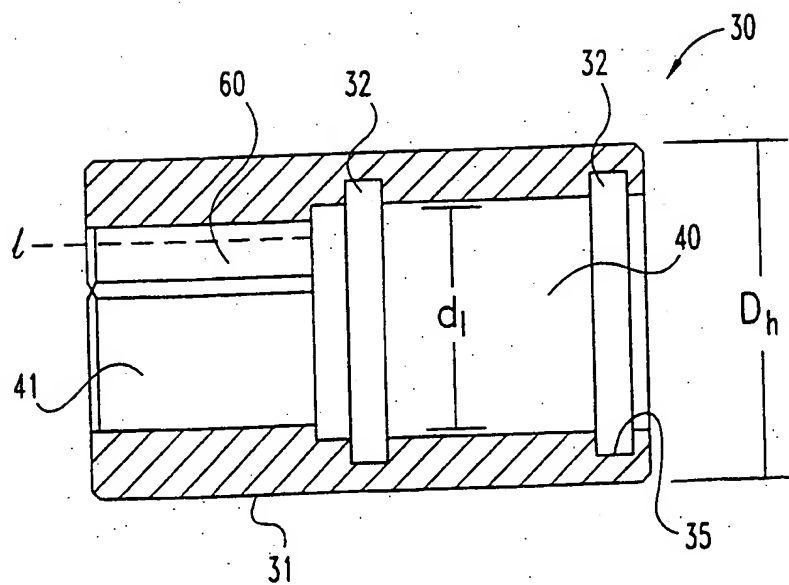


Fig. 3

3/21

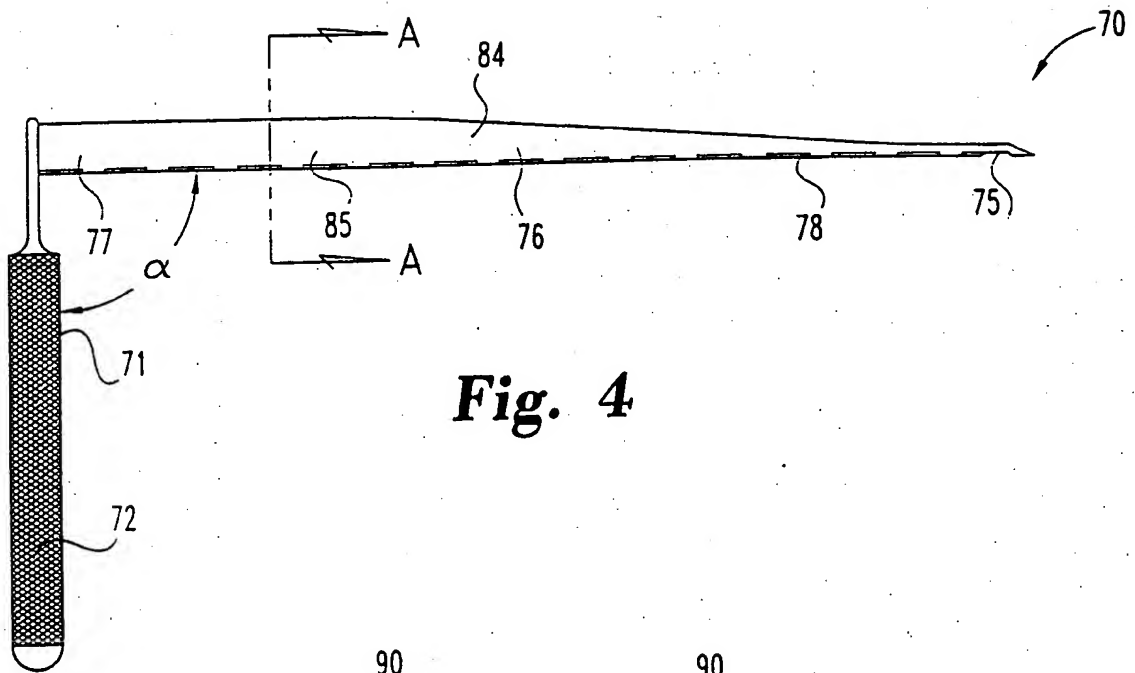


Fig. 4

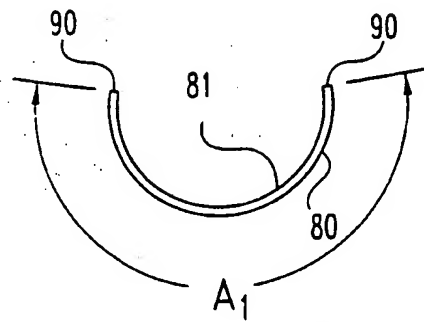


Fig. 4A

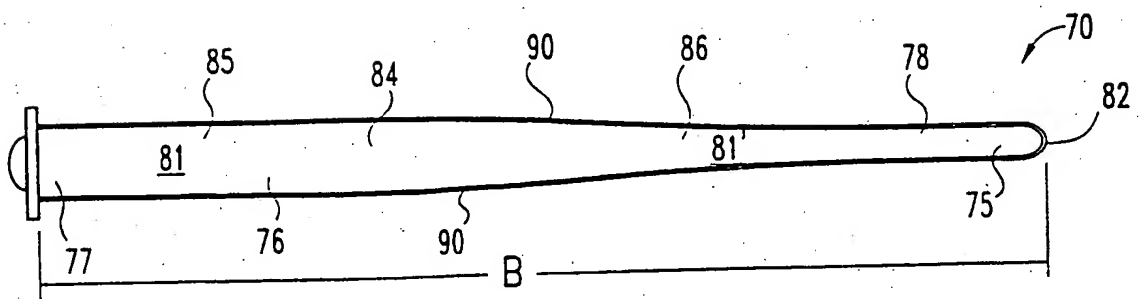


Fig. 5

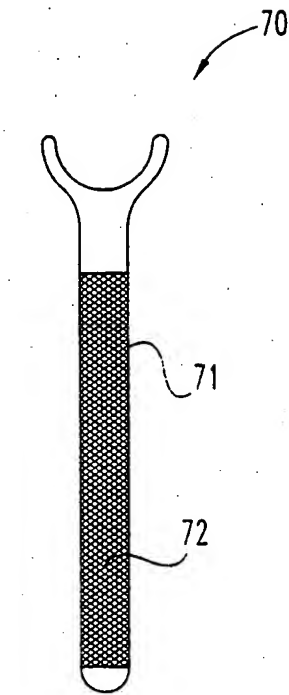


Fig. 6

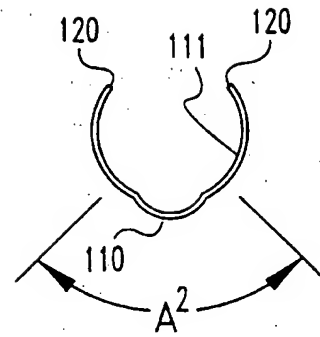


Fig. 7A

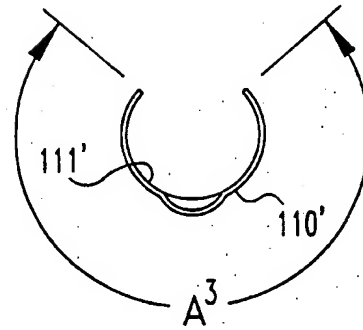


Fig. 7B

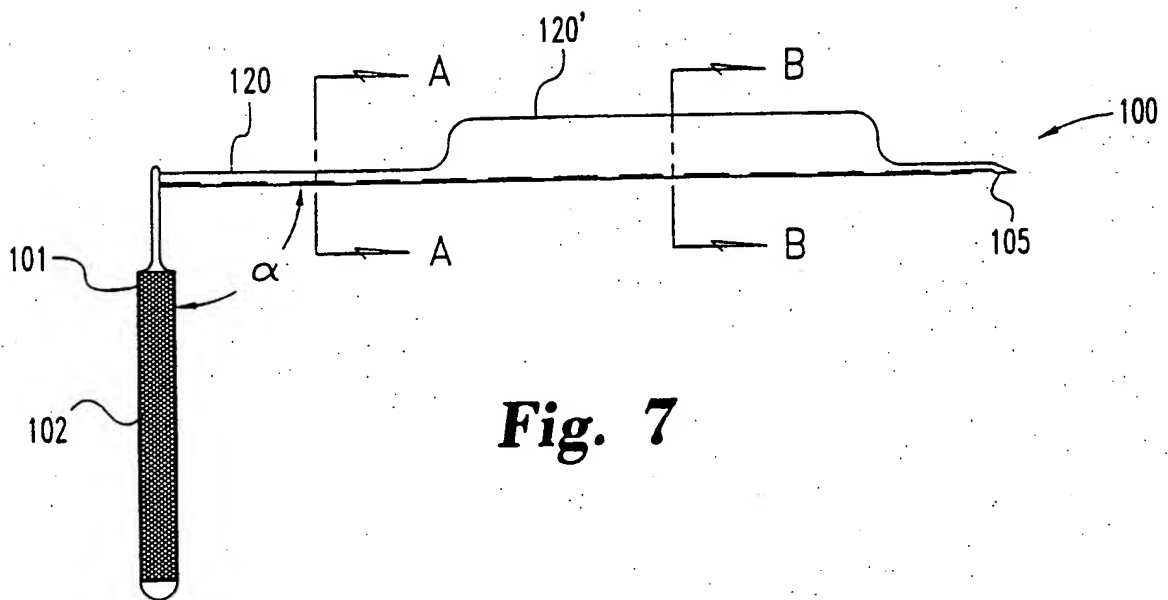


Fig. 7

5/21

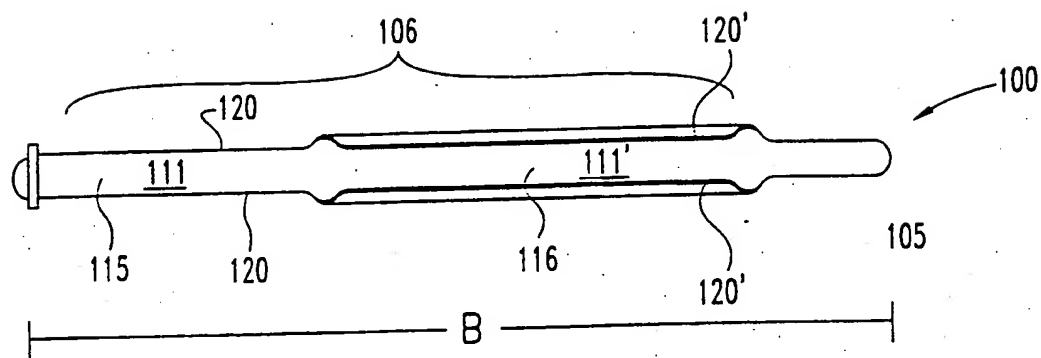


Fig. 8

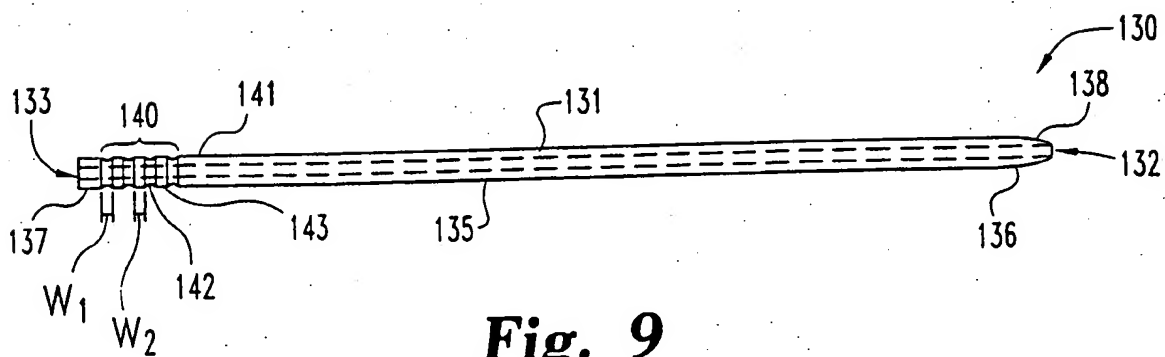


Fig. 9

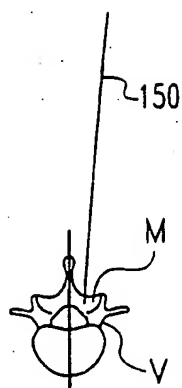


Fig. 10a

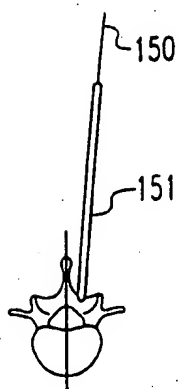


Fig. 10b

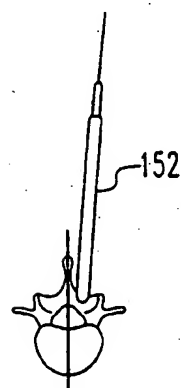


Fig. 10c

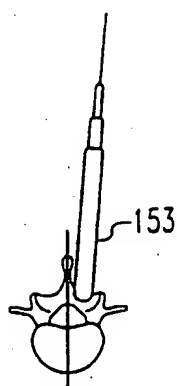


Fig. 10d

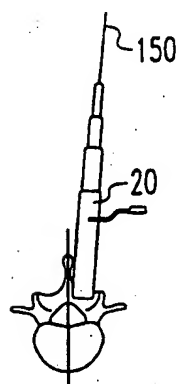


Fig. 10e




Fig. 10f




Fig. 10g

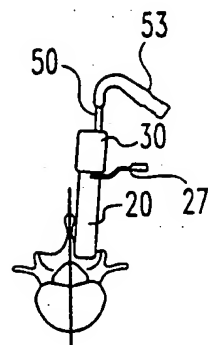


Fig. 10h

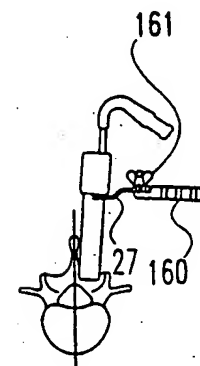


Fig. 10i

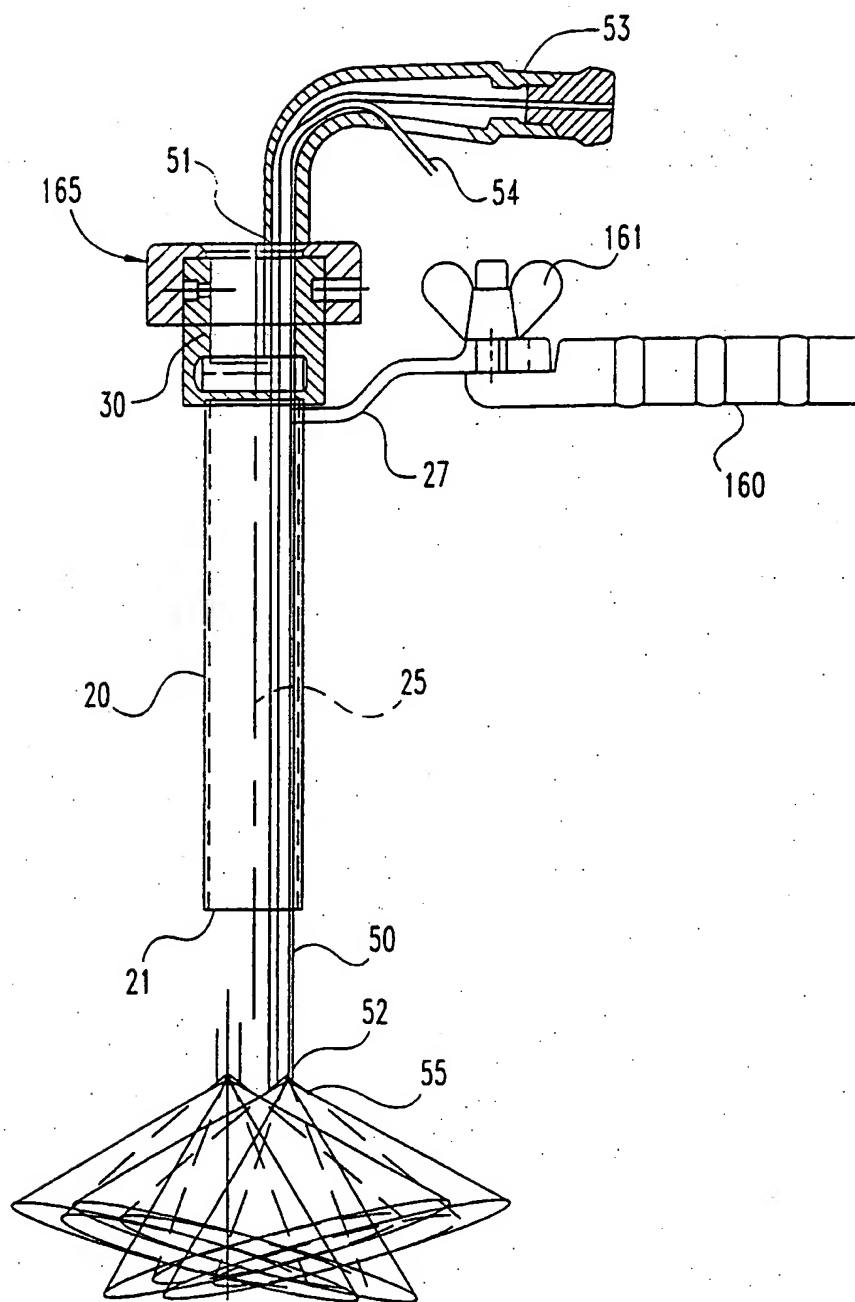


Fig. 11

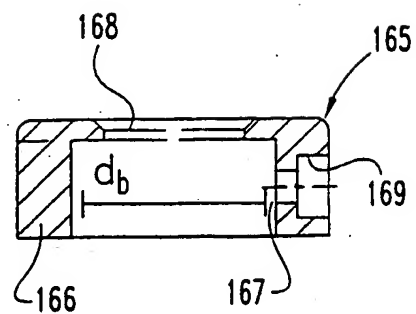


Fig. 12

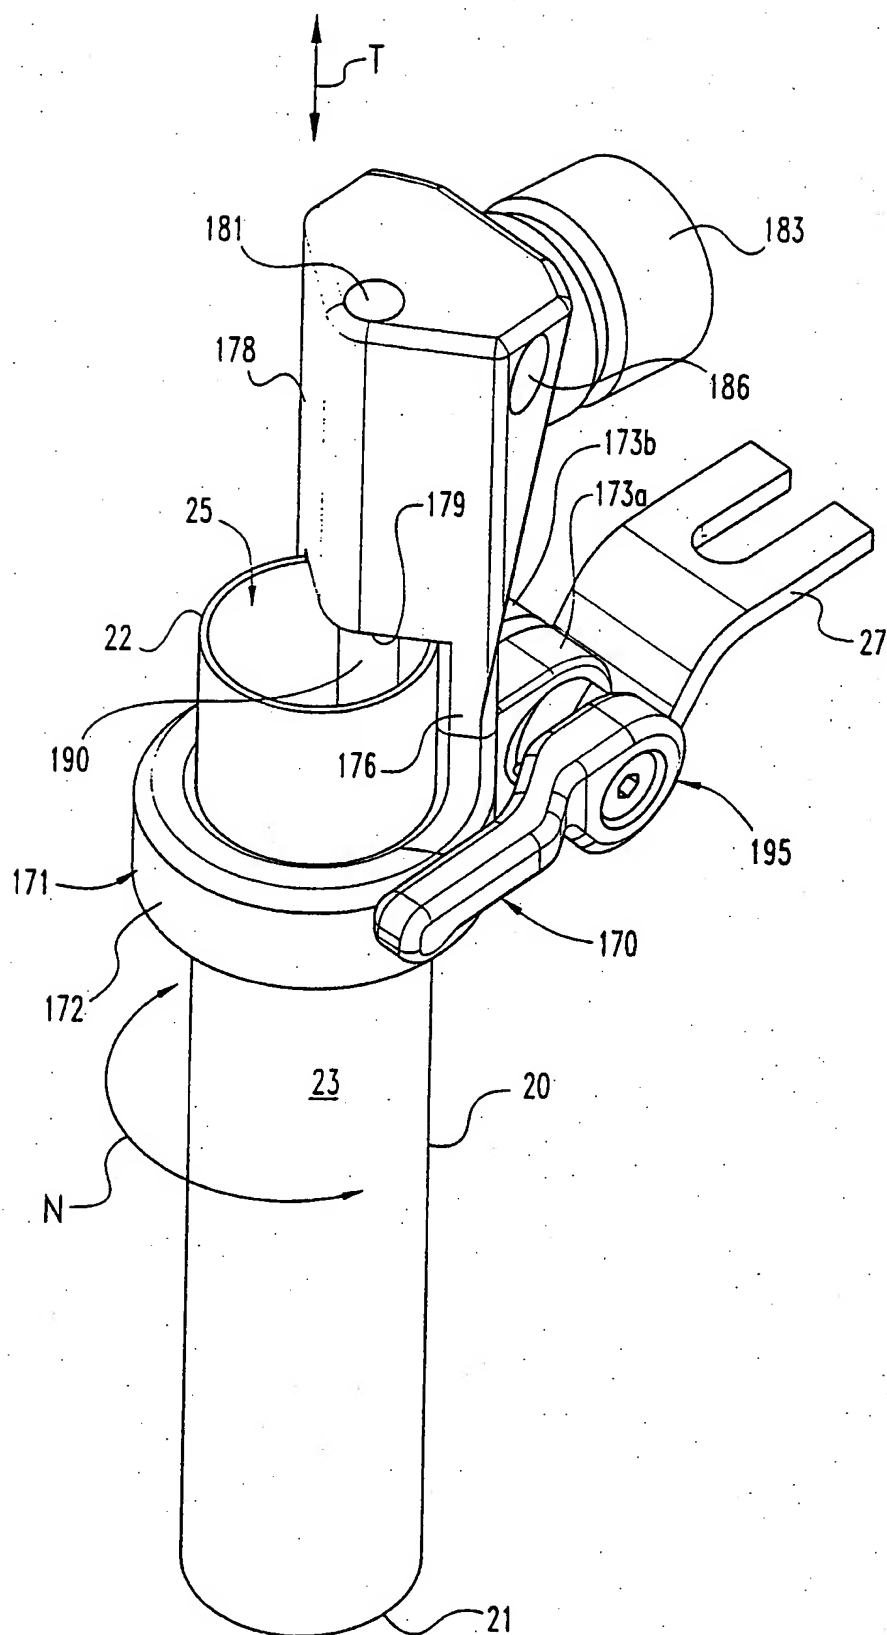
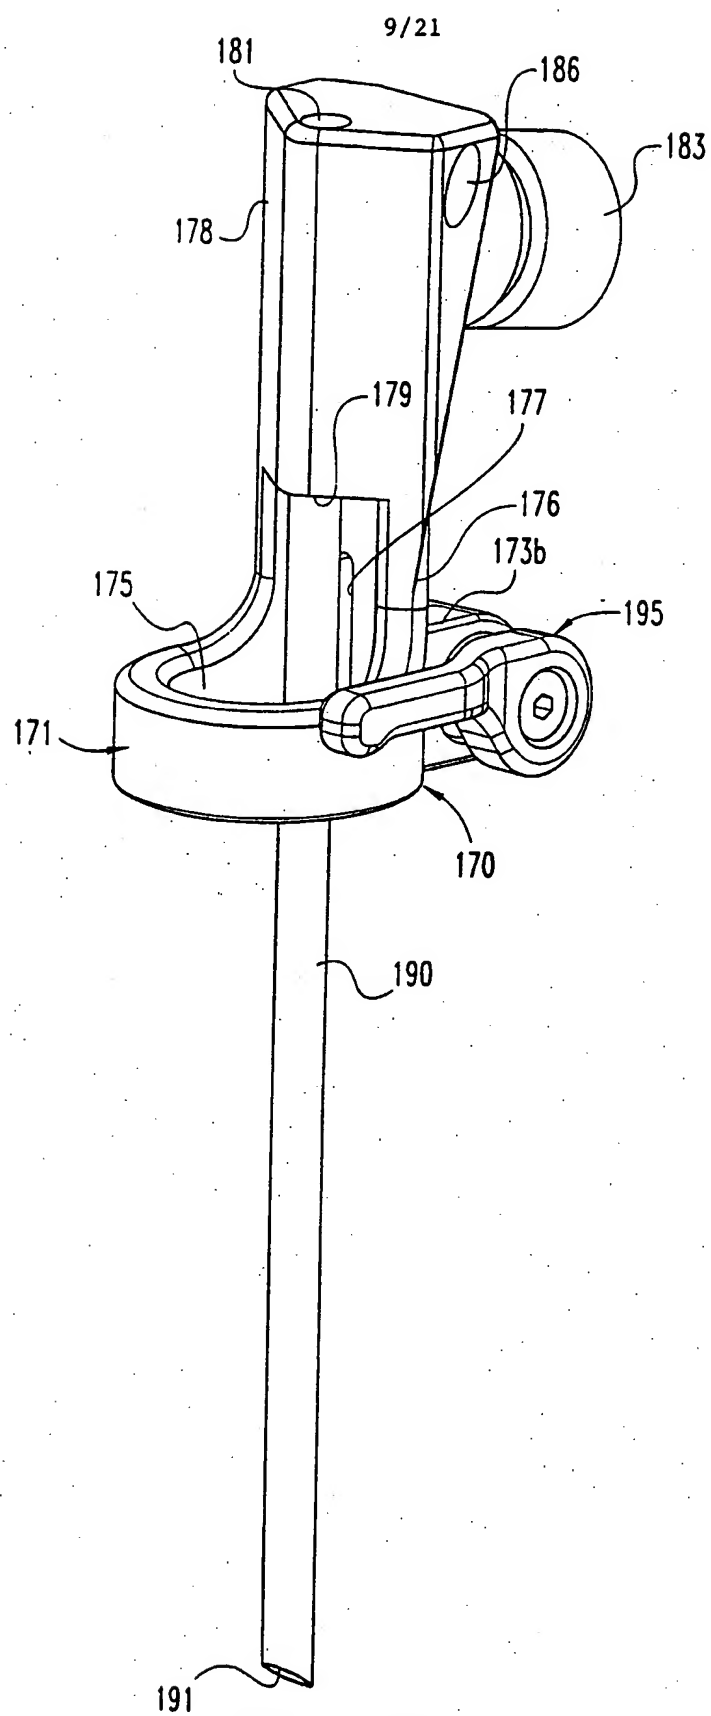


Fig. 13

**Fig. 14**

10/21

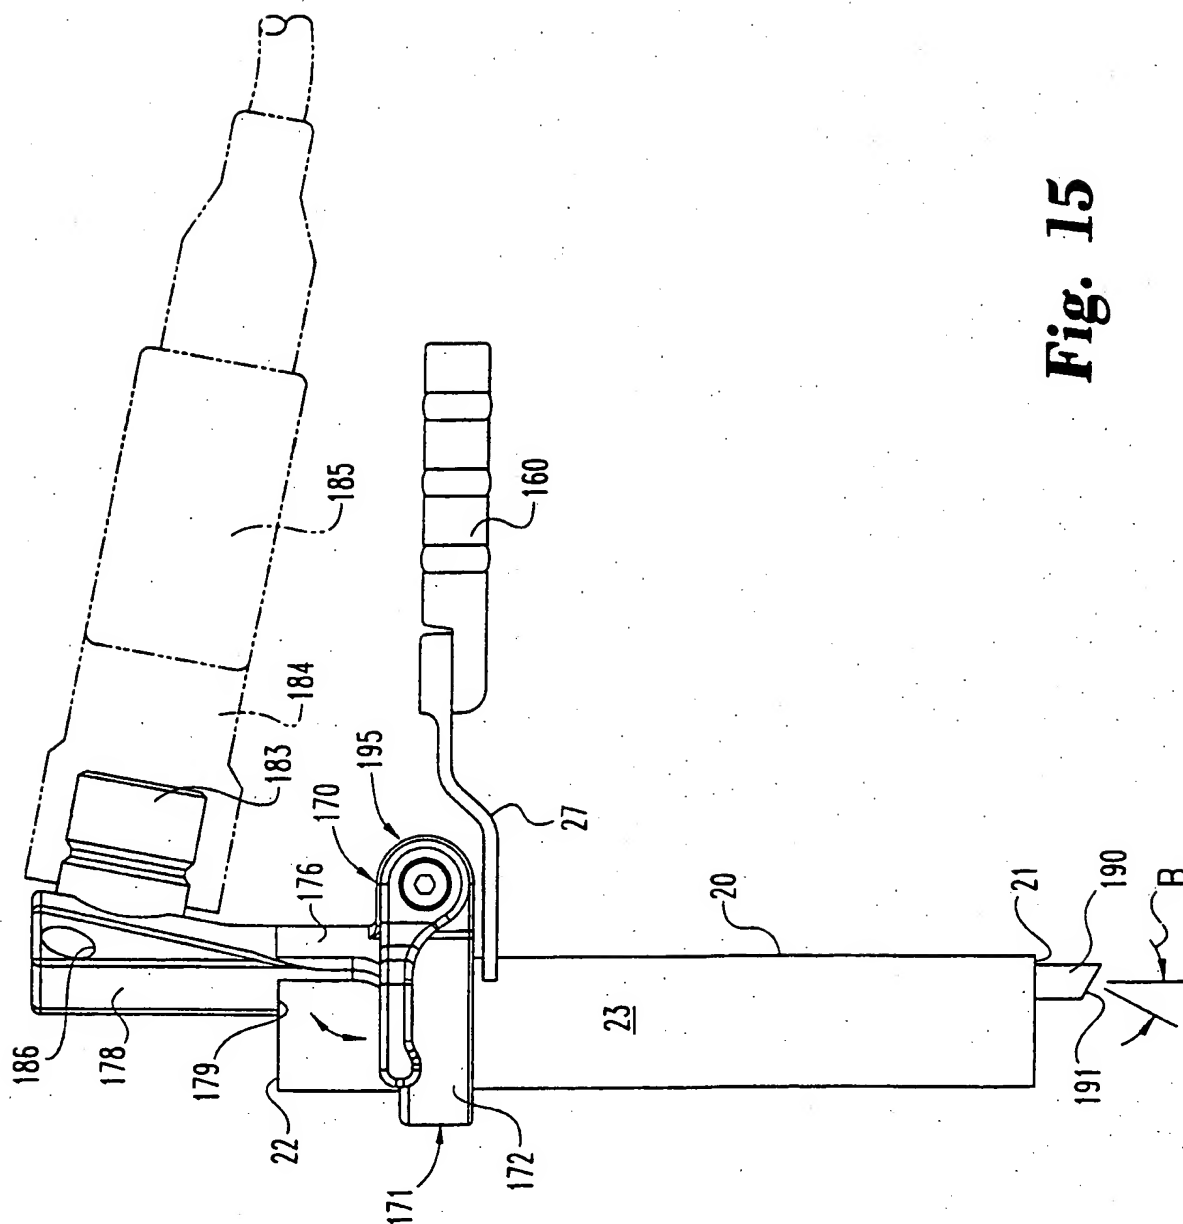


Fig. 15

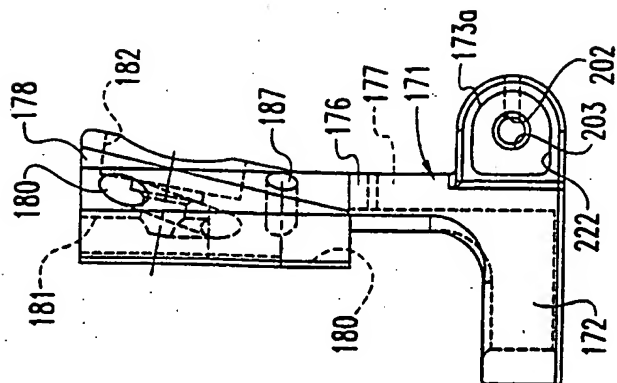


Fig. 16

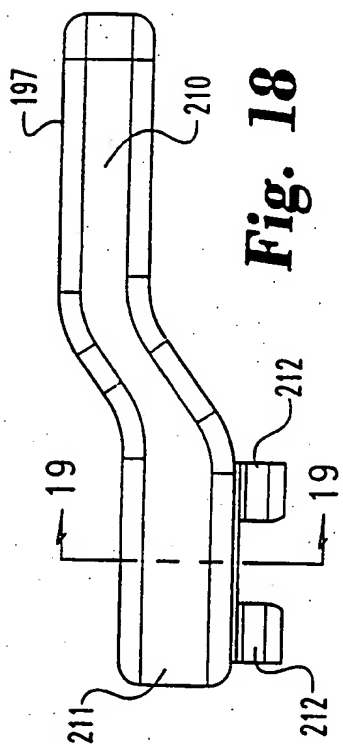


Fig. 18

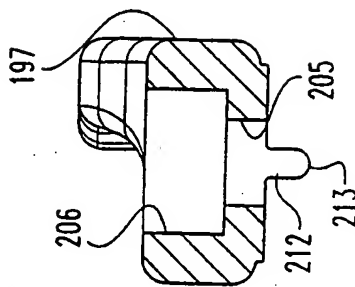


Fig. 19

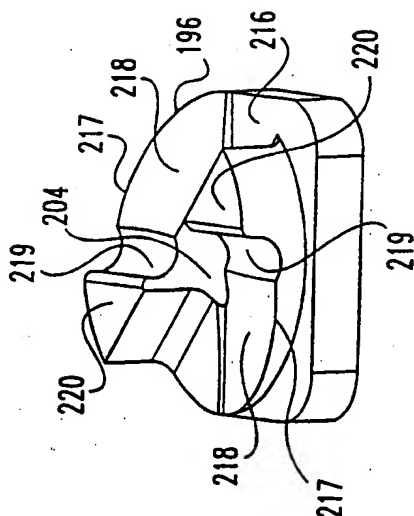


Fig. 20

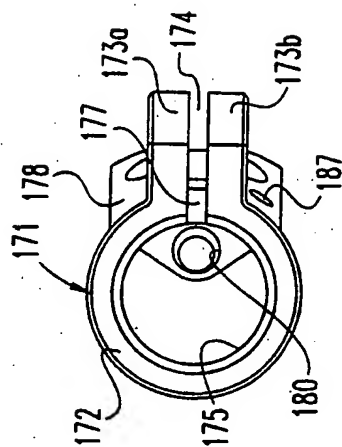


Fig. 21

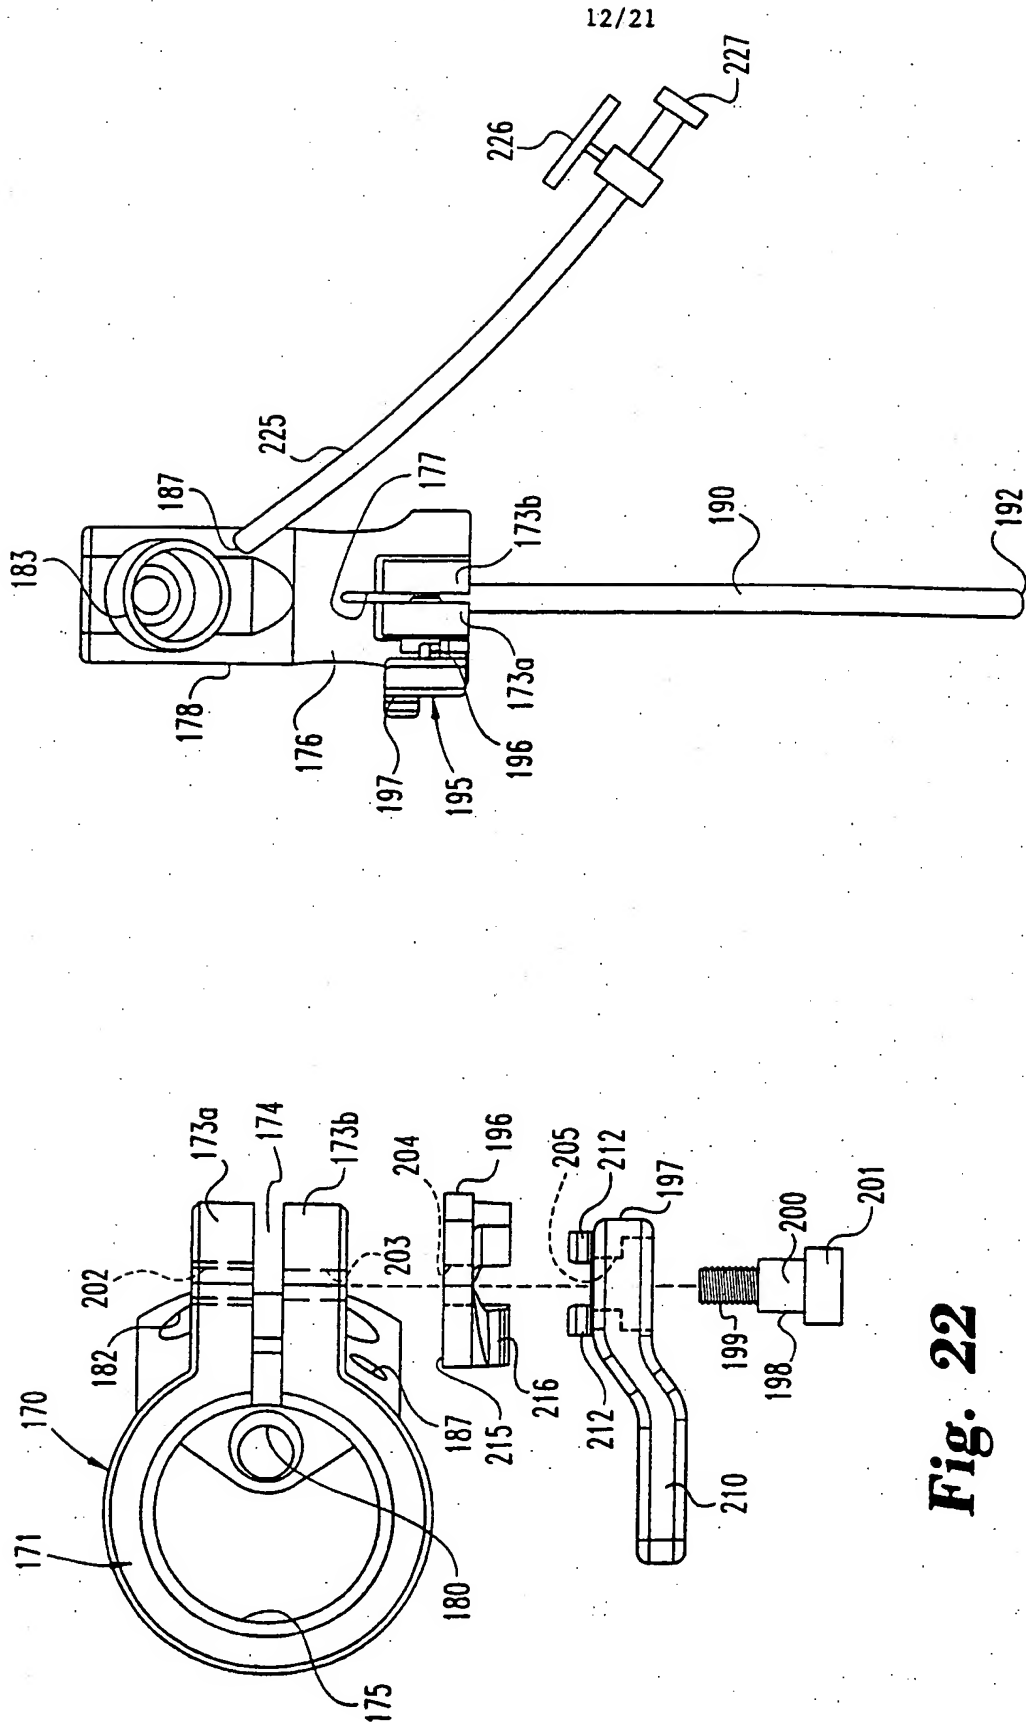



Fig. 23



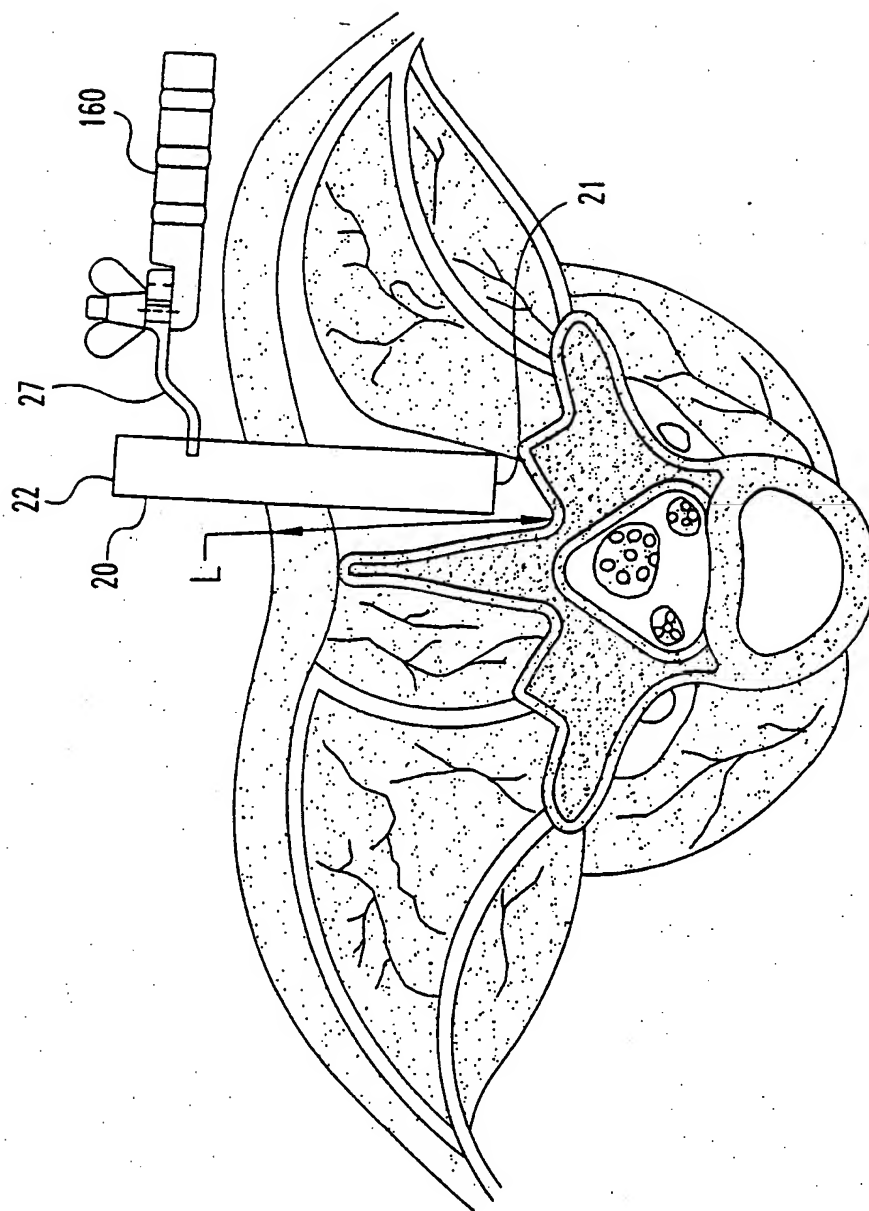


Fig. 24

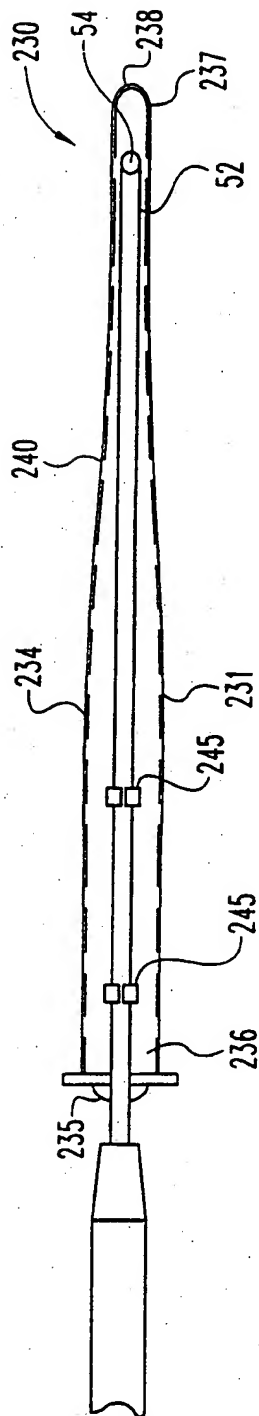


Fig. 26

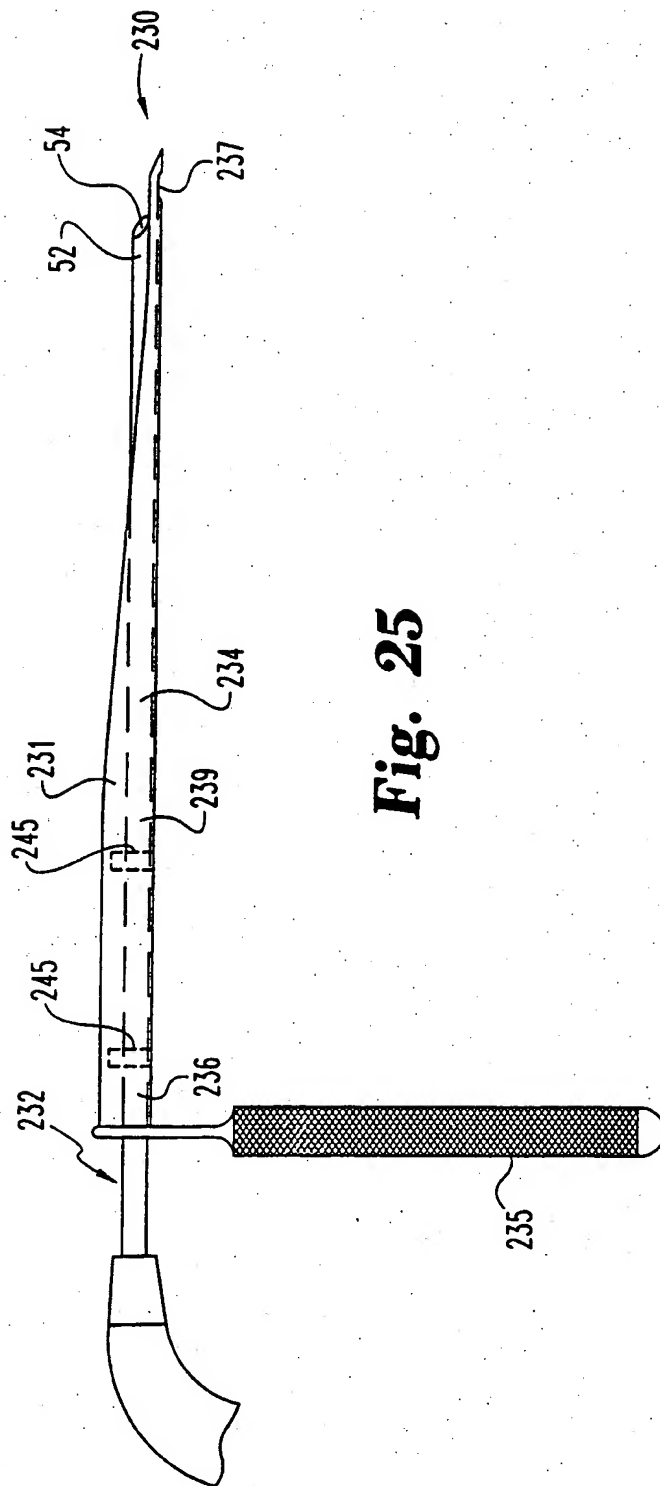
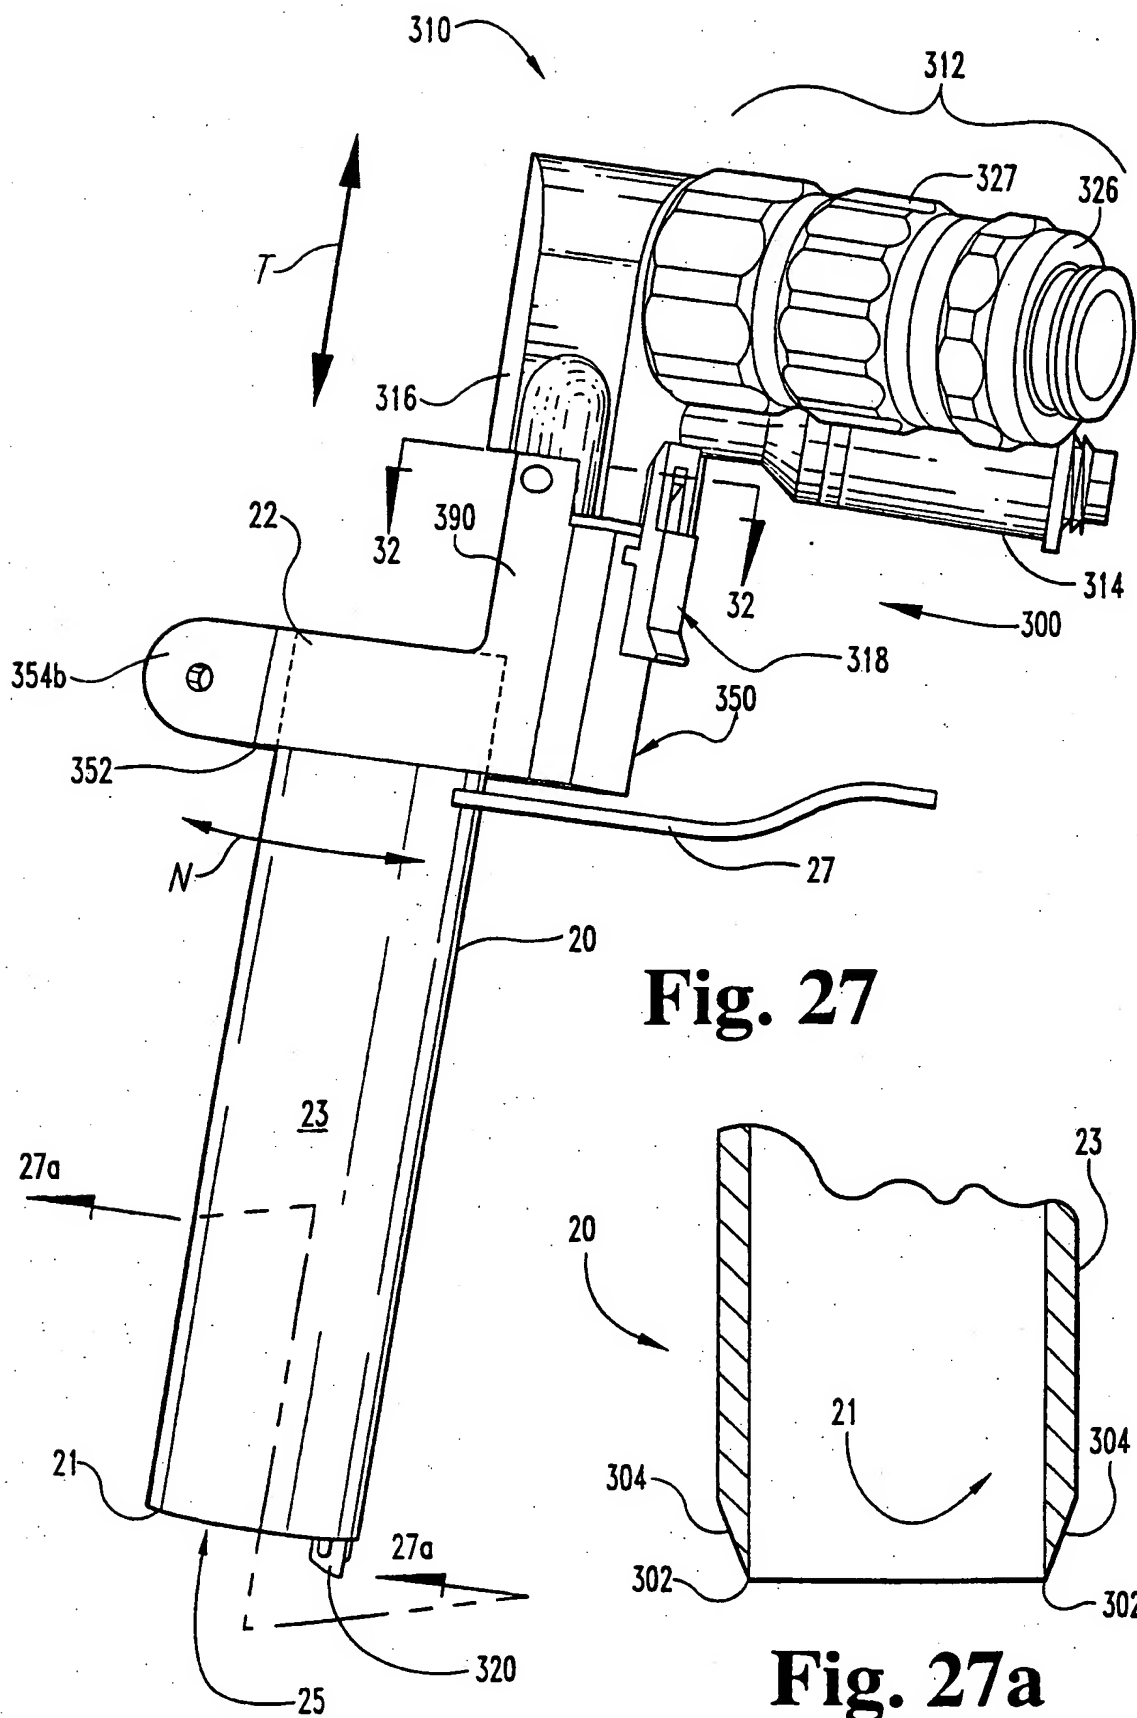
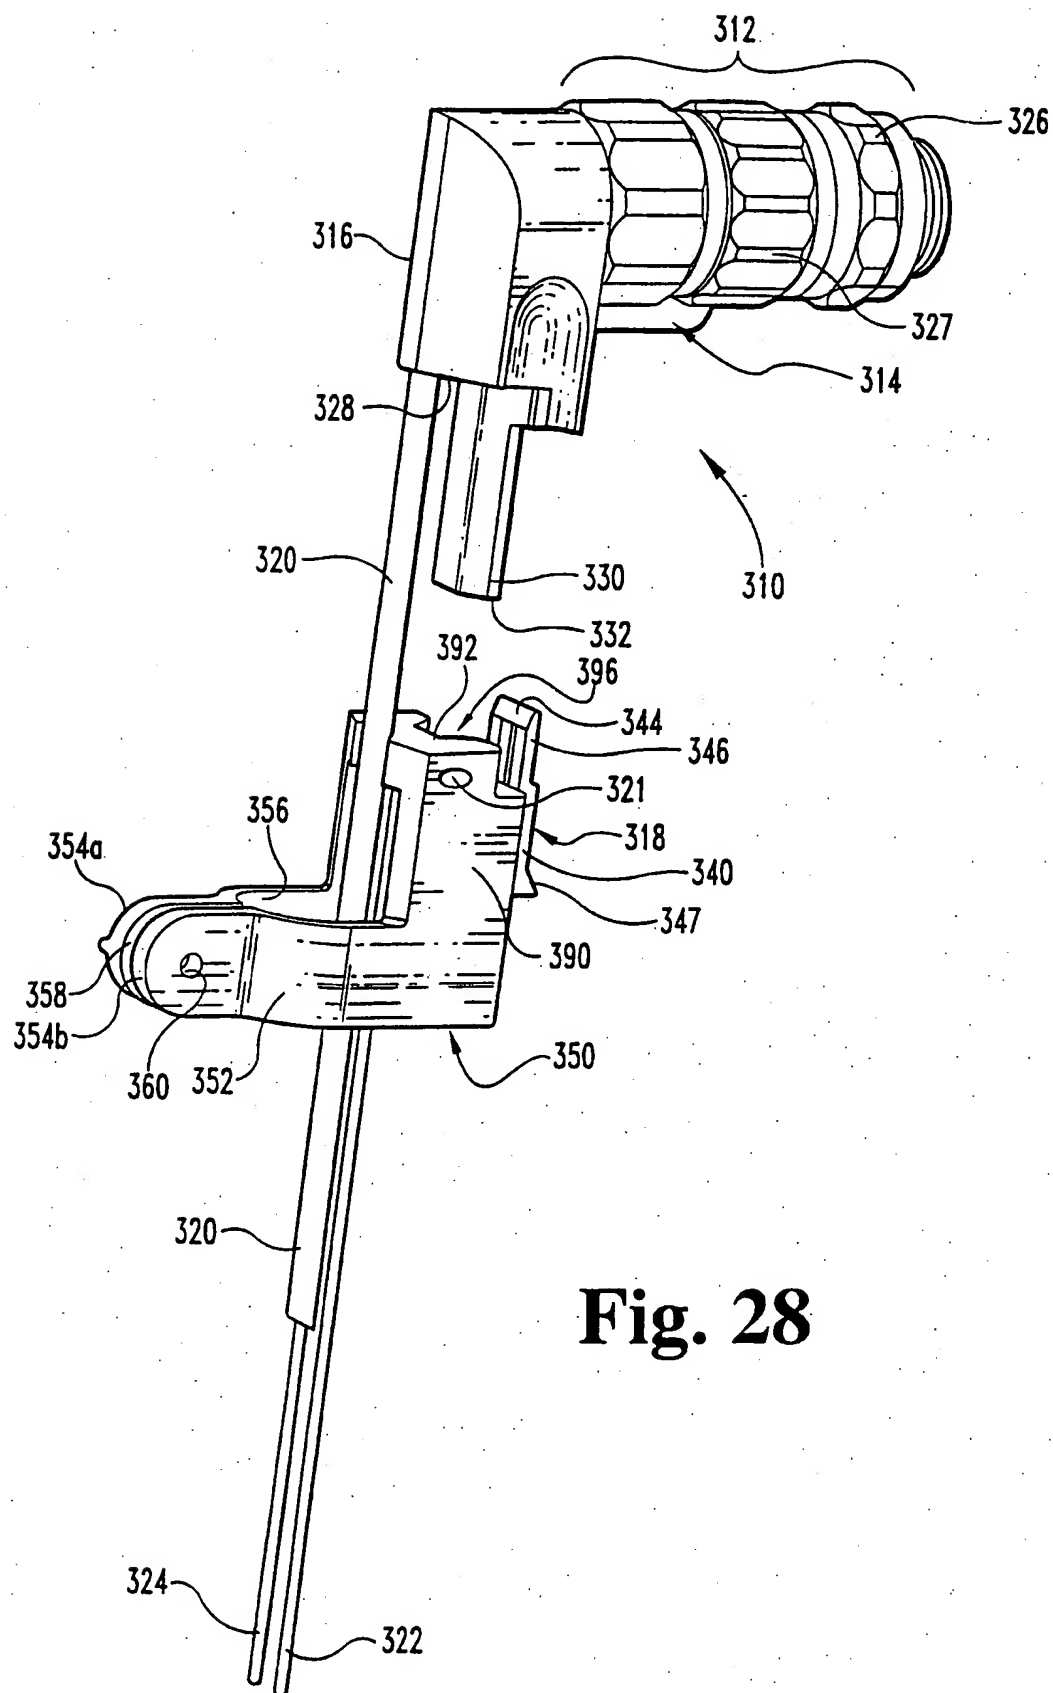
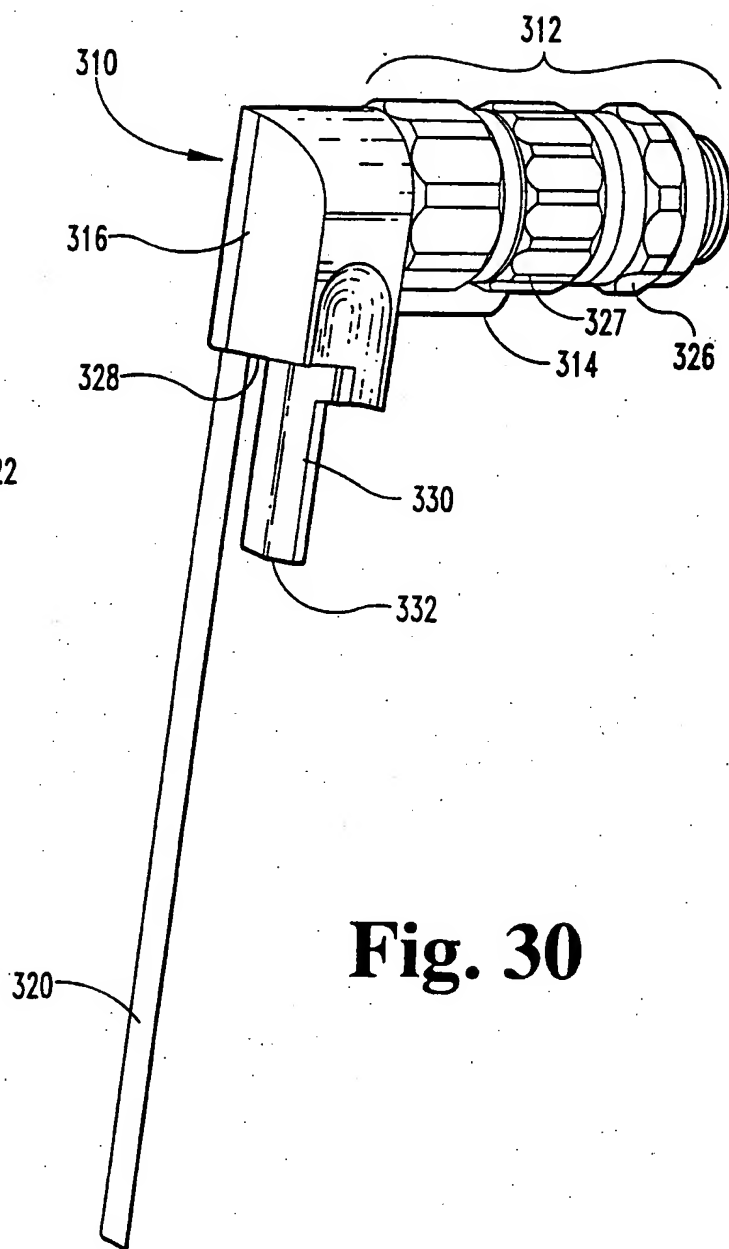
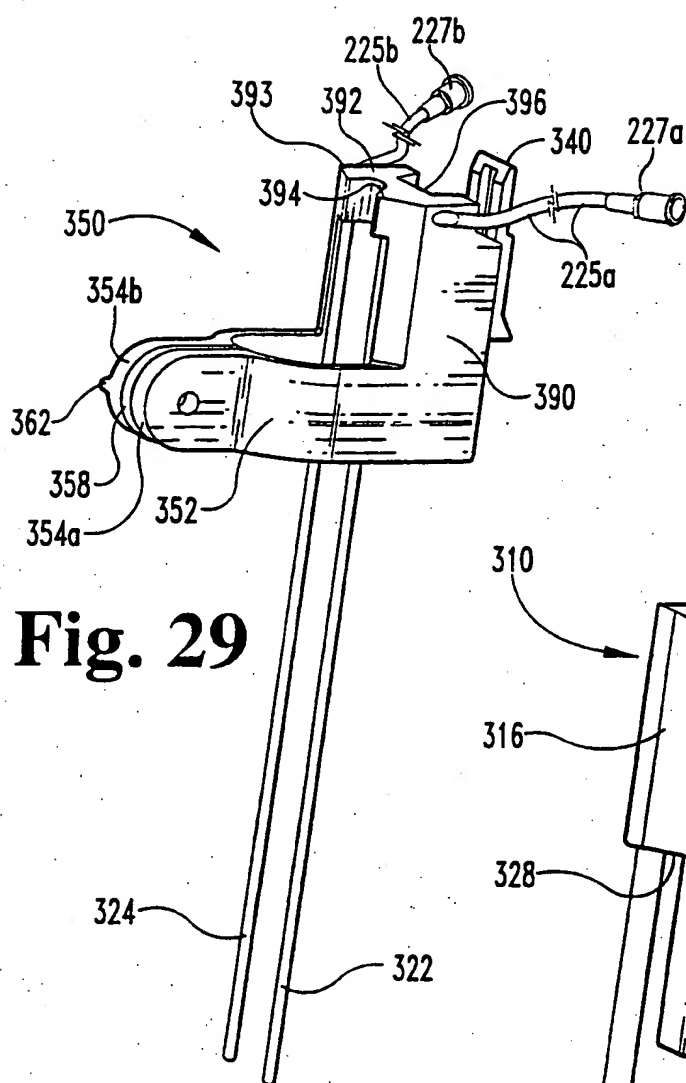


Fig. 25







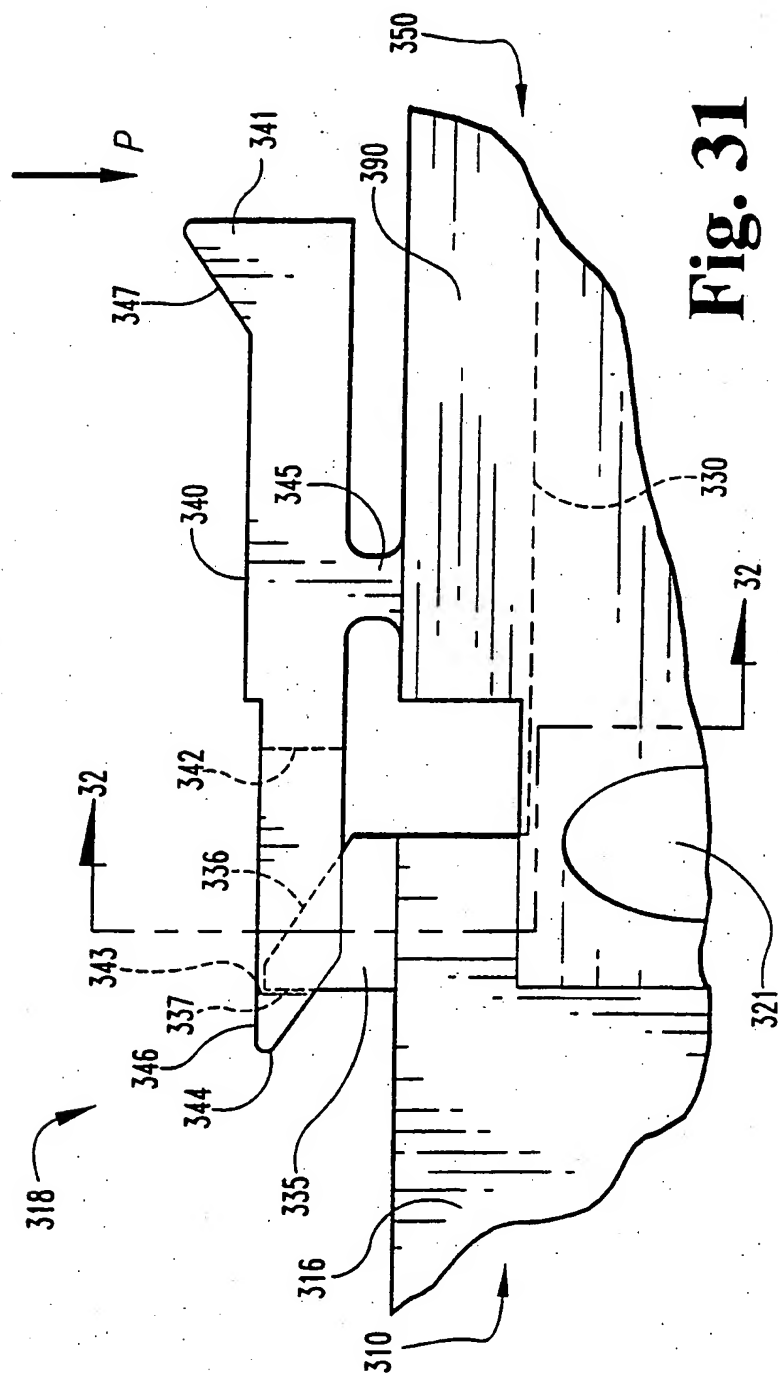
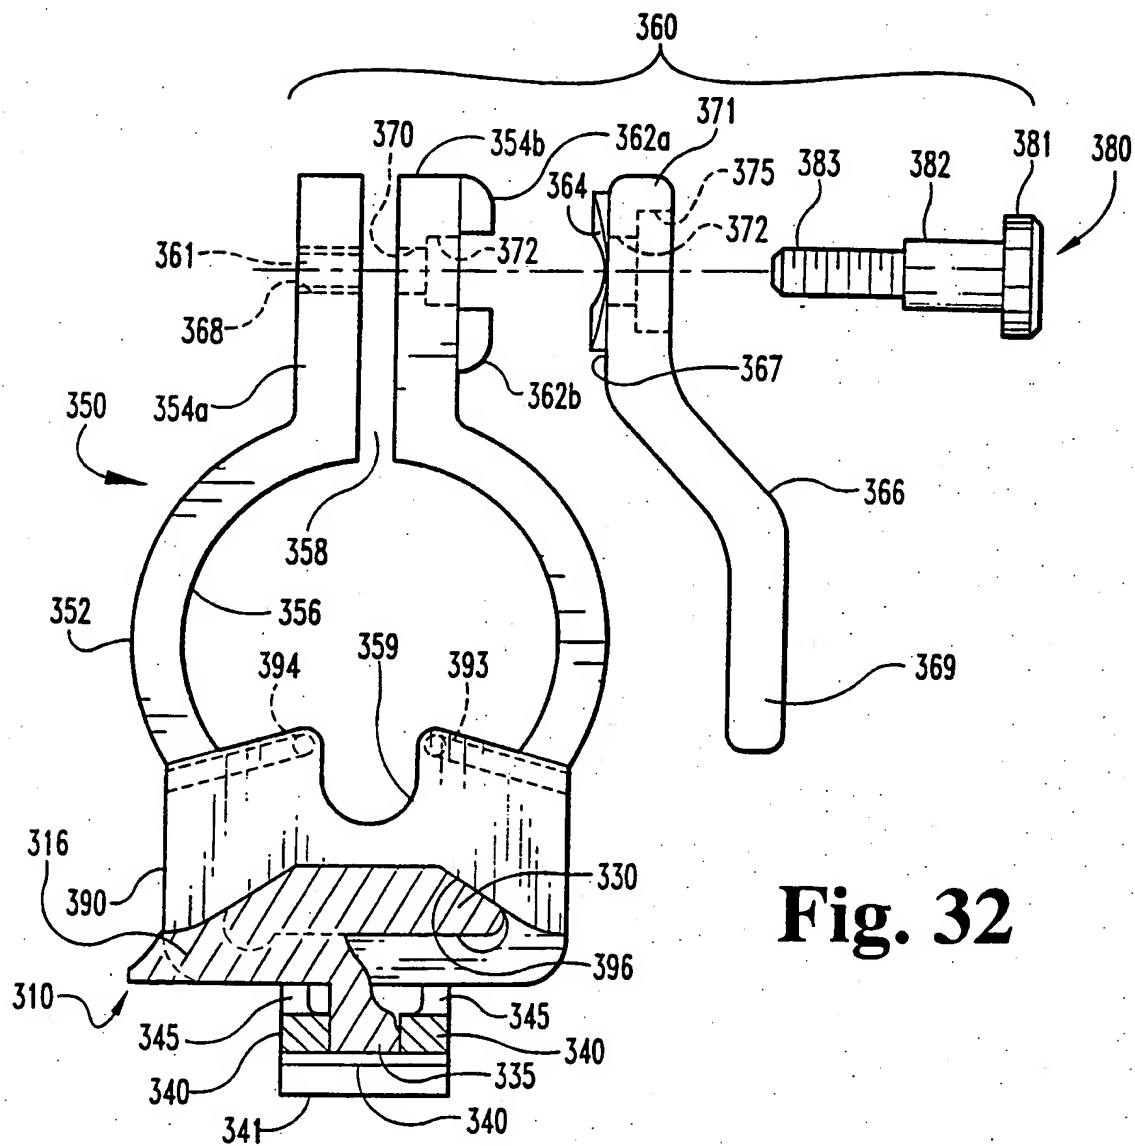


Fig. 31

**Fig. 32**

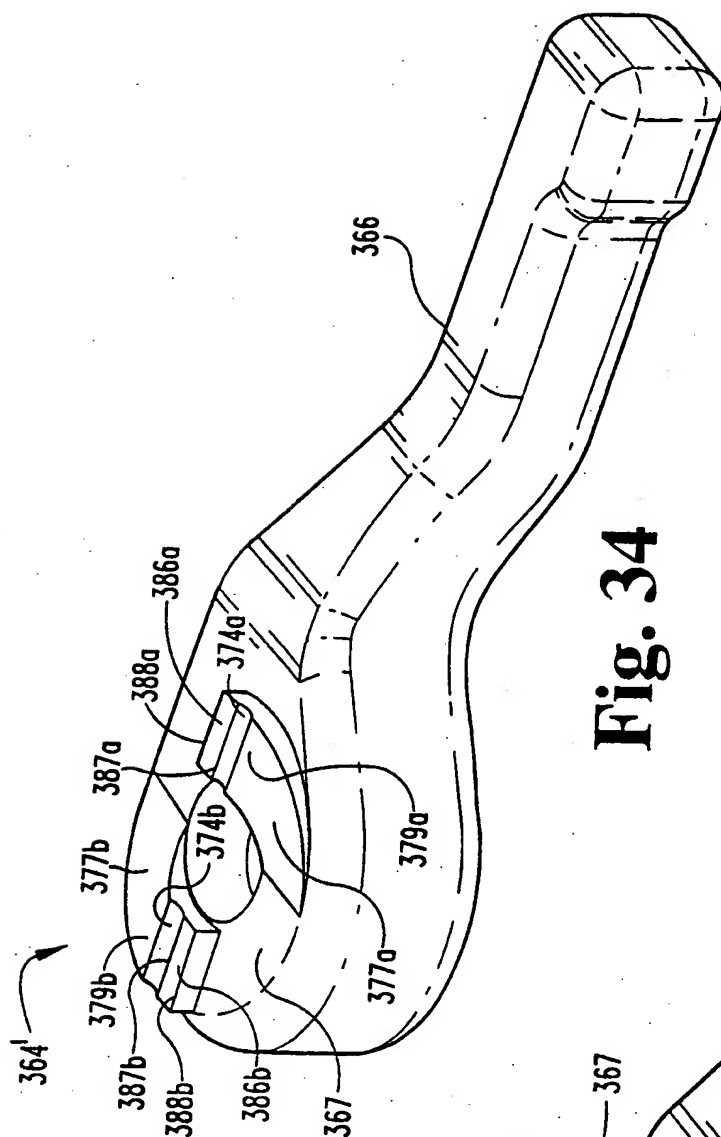


Fig. 34

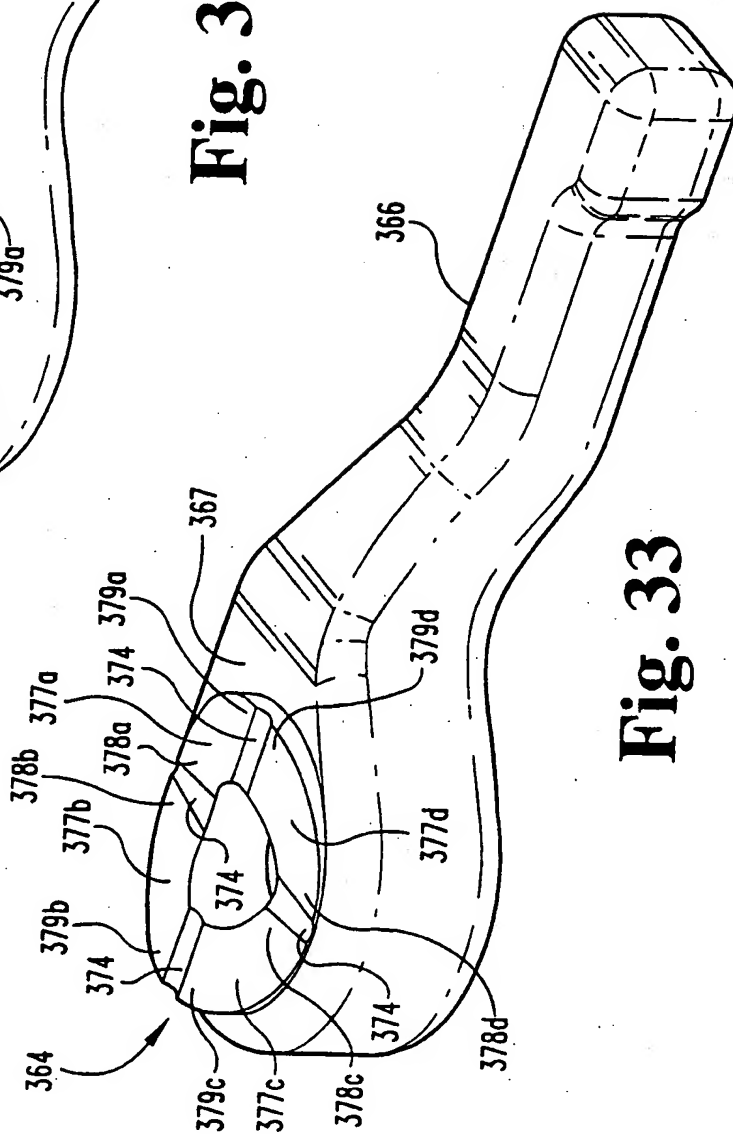


Fig. 33

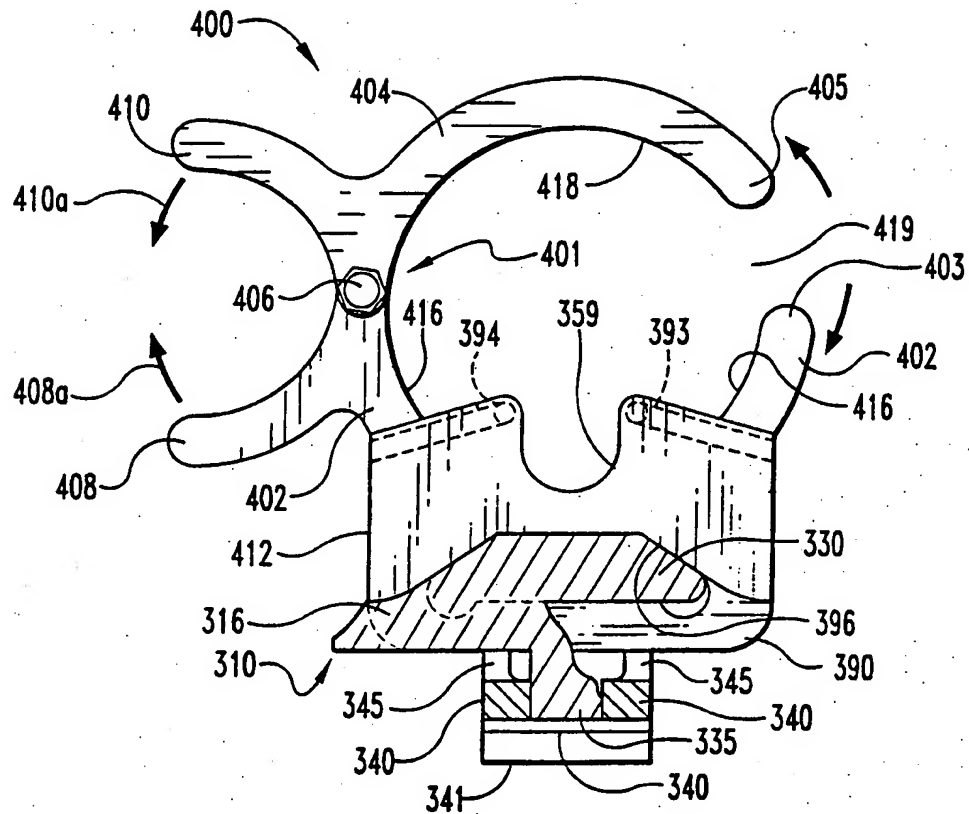


Fig. 35

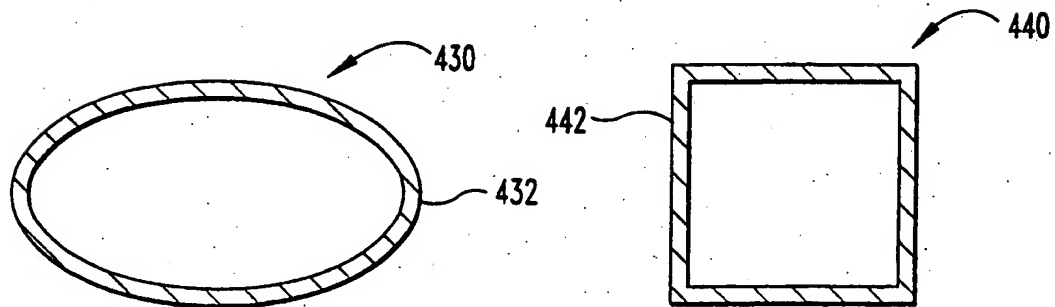


Fig. 36

Fig. 37

INTERNATIONAL SEARCH REPORT

Intern. Application No

PCT/US 99/21866

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61B17/34 A61M29/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61B A61M

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	<p>WO 97 34536 A (DANEK MEDICAL INC) 25 September 1997 (1997-09-25)</p> <p>page 35, line 25 - line 31; figures 15-24 -----</p>	<p>1,2,4,5, 7-19,22, 23,26-43</p>

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

8 December 1999

Date of mailing of the international search report

20/12/1999

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Gérard, B

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US 99/21866

Box I Observations where certain claims were found unsearchable (Continuation of item 1 of first sheet)

This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:

1. ☐ Claims Nos.:
because they relate to subject matter not required to be searched by this Authority, namely:
2. ☐ Claims Nos.:
because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. ☐ Claims Nos.:
because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).

Box II Observations where unity of invention is lacking (Continuation of item 2 of first sheet)

This International Searching Authority found multiple inventions in this international application, as follows:

see additional sheet

1. ☐ As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. ☒ As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. ☐ As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. ☐ No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the invention first mentioned in the claims; it is covered by claims Nos.:

Remark on Protest

- ☐ The additional search fees were accompanied by the applicant's protest.
- ☐ No protest accompanied the payment of additional search fees.

FURTHER INFORMATION CONTINUED FROM PCT/ISA/ 210

1. Claims: 1-39

Apparatus with clamp assembly connecting a viewing element

2. Claims: 40-43

Apparatus comprising a bracket and flexible arm mounted thereto

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 99/21866

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9734536 A	25-09-1997	US 5792044 A	11-08-1998
		US 5902231 A	11-05-1999
		AU 2324697 A	10-10-1997
		DE 19780707 T	02-07-1998
		EP 0891156 A	20-01-1999
		US 5954635 A	21-09-1999
<hr/>			